


**BioVendor**

Research  
and Diagnostic Products

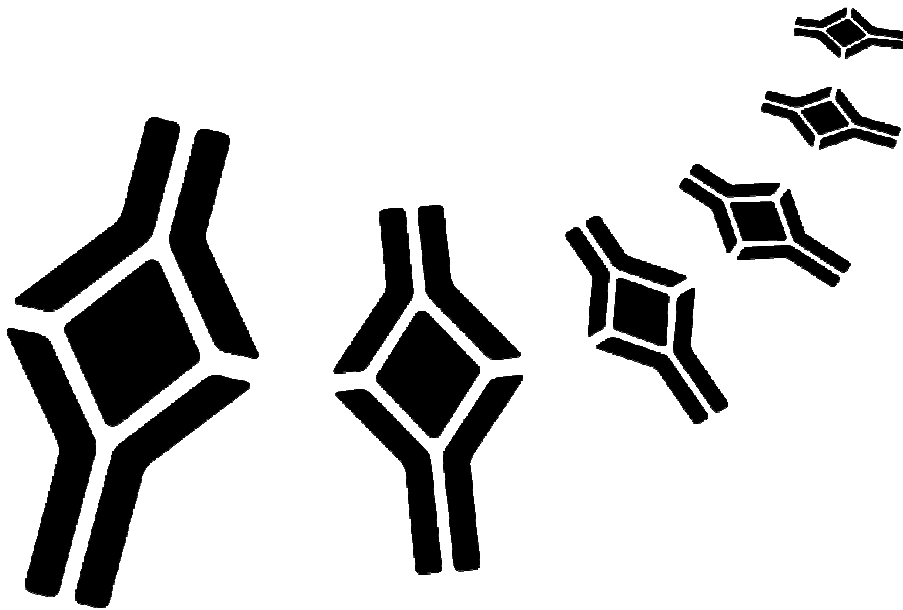

## **HUMAN ZINC-ALPHA-2-GLYCOPROTEIN ELISA**

**Product Data Sheet**

**Cat. No.: RD191093100R**

**For Research Use Only**

# CONTENTS

---

1.	INTENDED USE	3
2.	STORAGE, EXPIRATION	3
3.	INTRODUCTION	4
4.	TEST PRINCIPLE	5
5.	PRECAUTIONS	5
6.	TECHNICAL HINTS	6
7.	REAGENT SUPPLIED	6
8.	MATERIAL REQUIRED BUT NOT SUPPLIED	7
9.	PREPARATION OF REAGENTS	7
10.	PREPARATION OF SAMPLES	9
11.	ASSAY PROCEDURE	10
12.	CALCULATIONS	12
13.	PERFORMANCE CHARACTERISTICS	13
14.	DEFINITION OF THE STANDARD	17
15.	METHOD COMPARISON	17
16.	TROUBLESHOOTING AND FAQs	17
17.	REFERENCES	18
18.	EXPLANATION OF SYMBOLS	21

**»» This kit is manufactured by:  
BioVendor – Laboratorní medicína a.s.**

**»» Use only the current version of Product Data Sheet enclosed with the kit!**

## 1. INTENDED USE

---

The RD191093100R Human Zinc-Alpha-2-Glycoprotein ELISA is a sandwich enzyme immunoassay for the quantitative measurement of human zinc-alpha-2-glycoprotein.

### »» Features

- **It is intended for research use only**
- The total assay time is less than 3 hours
- The kit measures zinc-alpha-2-glycoprotein in serum and plasma (EDTA, citrate, heparin)
- Assay format is 96 wells
- Quality Controls are human serum based. No animal sera are used
- Standard is recombinant protein based
- Components of the kit are provided ready to use, concentrated or lyophilized

## 2. STORAGE, EXPIRATION

---

Store the complete kit at 2-8°C. Under these conditions, the kit is stable until the expiration date (see label on the box).

For stability of opened reagents see Chapter 9.

### 3. INTRODUCTION

---

Zinc-alpha-2-glycoprotein (ZAG, ZA2G, Azgp1, ZNGP1, Lipid-Mobilizing Factor, LMF) is a soluble 41kDa glycoprotein belonging to the immunoglobulin protein family and consisting of a single polypeptide chain. Human ZAG shares 59% sequence identity with the murine homolog. ZAG is closely related to antigens of the class1 major histocompatibility complex (MHC I) and shares 30-40% sequence identity with the heavy chain of MHC I. Most MHC-I members heterodimerize with beta-2-microglobuline (b2m) and bind peptides derived from intracellular proteins to present them to cytotoxic T cells. In contrast, ZAG is a soluble protein rather than being anchored to plasma membranes that acts independently on b2m and binds the hydrophobic ligand, which may relate to its function in lipid metabolism.

ZAG is widespread in body fluids and is also found in various human tissues such as adipose tissue, prostate, breast, skin, salivary gland, trachea, broncheus, lung, gastrointestinal tract, pancreas, liver and kidney. ZAG acts as a lipid mobilizing factor to induce lipolysis in adipocytes and plays an important role in lipid utilization and loss of adipose tissue, especially during cachexia, which occurs in patient suffering from cancer, AIDS and other chronic illnesses. The role of ZAG in cancer cachexia is also connected with its ability to directly influence expression of uncoupling proteins (UCPs), which are implicated in the regulation of energy balance. In human adipocytes, ZAG expression is regulated particularly through TNF-alpha and the PPAR gamma nuclear receptor. ZAG expression is also upregulated by glucocorticoides and attenuated by eicosapentaenoic acid (EPA) and beta-3-adrenoreceptor antagonists.

ZAG is overexpressed in certain human malignant tumors such as prostate, breast, lung or bladder cancer and can relate to tumor differentiation. Additionally, ZAG plays a role in obesity, diabetic kidney disorders, frontotemporal dementia and regulation of melanin production by melanocytes.

ZAG is proposed to have a therapeutic use in obesity and cachexia. It can be used as a marker for clinical analysis of diabetic nephropathy and as a marker for certain tumors.

#### Areas of investigation:

Energy metabolism and body weight regulation

Oncology

## 4. TEST PRINCIPLE

---

In the BioVendor Human Zinc-Alpha-2-Glycoprotein (ZA2G) ELISA, standards, quality controls and samples are incubated in microplate wells pre-coated with polyclonal anti-human ZA2G antibody. After 60 minutes incubation and washing, polyclonal anti-human ZA2G antibody, conjugated with horseradish peroxidase (HRP) is added to the wells and incubated for 60 minutes with captured ZA2G. Following another washing step, the remaining HRP conjugate is allowed to react with the substrate solution (TMB). The reaction is stopped by addition of acidic solution and absorbance of the resulting yellow product is measured. The absorbance is proportional to the concentration of ZA2G. A standard curve is constructed by plotting absorbance values against concentrations of standards, and concentrations of unknown samples are determined using this standard curve.

## 5. PRECAUTIONS

---

- **For professional use only**
- Wear gloves and laboratory coats when handling immunodiagnostic materials
- Do not drink, eat or smoke in the areas where immunodiagnostic materials are being handled
- This kit contains components of human origin. These materials were found non-reactive for HBsAg, HCV antibody and for HIV 1/2 antigen and antibody. However, these materials should be handled as potentially infectious, as no test can guarantee the complete absence of infectious agents
- Avoid contact with the acidic Stop Solution and Substrate Solution, which contains hydrogen peroxide and tetramethylbenzidine (TMB). Wear gloves and eye and clothing protection when handling these reagents. Stop and/or Substrate Solutions may cause skin/eyes irritation. In case of contact with the Stop Solution and the Substrate Solution wash skin/eyes thoroughly with water and seek medical attention, when necessary
- The materials must not be pipetted by mouth

## 6. TECHNICAL HINTS

---

- Reagents with different lot numbers should not be mixed
- Use thoroughly clean glassware
- Use deionized (distilled) water, stored in clean containers
- Avoid any contamination among samples and reagents. For this purpose, disposable tips should be used for each sample and reagent
- Substrate Solution should remain colourless until added to the plate. Keep Substrate Solution protected from light
- Stop Solution should remain colourless until added to the plate. The colour developed in the wells will turn from blue to yellow immediately after the addition of the Stop Solution. Wells that are green in colour indicate that the Stop Solution has not mixed thoroughly with the Substrate Solution
- Dispose of consumable materials and unused contents in accordance with applicable national regulatory requirements

## 7. REAGENT SUPPLIED

---

<i>Kit Components</i>	<i>State</i>	<i>Quantity</i>
Antibody Coated Microtiter Strips	ready to use	96 wells
Conjugate Solution	ready to use	13 ml
Master Standard	lyophilized	1 vial
Quality Control HIGH	lyophilized	1 vial
Quality Control LOW	lyophilized	1 vial
Dilution Buffer Conc. (2x)	concentrated	50 ml
Wash Solution Conc. (10x)	concentrated	100 ml
Substrate Solution	ready to use	13 ml
Stop Solution	ready to use	13 ml
Product Data Sheet + Certificate of Analysis	-	1 pc

## 8. MATERIAL REQUIRED BUT NOT SUPPLIED

---

- Deionized (distilled) water
- Test tubes for diluting samples
- Glassware (graduated cylinder and bottle) for Wash Solution (Dilution Buffer)
- Precision pipettes to deliver 5-1000  $\mu$ l with disposable tips
- Multichannel pipette to deliver 100  $\mu$ l with disposable tips
- Absorbent material (e.g. paper towels) for blotting the microtiter plate after washing
- Vortex mixer
- Orbital microplate shaker capable of approximately 300 rpm
- Microplate washer (optional). [Manual washing is possible but not preferable.]
- Microplate reader with  $450 \pm 10$  nm filter, preferably with reference wavelength 630 nm (alternatively another one from the interval 550-650 nm)
- Software package facilitating data generation and analysis (optional)

## 9. PREPARATION OF REAGENTS

---

- All reagents need to be brought to room temperature prior to use
- Always prepare only the appropriate quantity of reagents for your test
- Do not use components after the expiration date marked on their label
- Assay reagents supplied ready to use:

### **Antibody Coated Microtiter Strips**

#### Stability and storage:

Return the unused strips to the provided aluminium zip-sealed bag with desiccant and seal carefully. Remaining Microtiter Strips are stable 3 months when stored at 2-8°C and protected from the moisture.

### **Conjugate Solution**

### **Substrate Solution**

### **Stop Solution**

#### Stability and storage:

Opened reagents are stable 3 months when stored at 2-8°C.

- **Assay reagents supplied concentrated or lyophilized:**

**Dilution Buffer Conc. (2x)**

Dilute Dilution Buffer Concentrate (2x) two-fold in distilled water to prepare a 1x working solution. Example: 50 ml of Dilution Buffer Concentrate (2x) + 50 ml of distilled water for use of all 96-wells.

Stability and storage:

The diluted Dilution Buffer is stable 1 month when stored at 2-8°C. Opened Dilution Buffer Concentrate (2x) is stable 3 months when stored at 2-8°C.

**Human Zinc-Alpha-2-Glycoprotein Master Standard**

**Refer to the Certificate of Analysis for current volume of Dilution Buffer needed for reconstitution of standard!!!**

Reconstitute the lyophilized Master Standard with Dilution Buffer just prior to the assay. Let it dissolve at least 15 minutes with occasional gentle shaking (not to foam). The resulting concentration of the Human ZA2G in the stock solution is **100 ng/ml**.

Prepare set of standards using Dilution Buffer as follows:

<i>Volume of Standard</i>	<i>Dilution Buffer</i>	<i>Concentration</i>
Stock	-	100 ng/ml
250 µl of stock	250 µl	50 ng/ml
250 µl of 50 ng/ml	250 µl	25 ng/ml
<b>240 µl of 25 ng/ml</b>	<b>260 µl</b>	12 ng/ml
250 µl of 12 ng/ml	250 µl	6 ng/ml
250 µl of 6 ng/ml	250 µl	3 ng/ml

**Prepared Standards are ready to use, do not dilute them.**

Stability and storage:

Standard stock solution (100 ng/ml) should be aliquoted and frozen at -20°C for 3 months. Avoid repeated freeze/thaw cycles.

**Do not store the diluted Standard solutions.**

**Quality Controls HIGH, LOW**

**Refer to the Certificate of Analysis for current volume of Dilution Buffer needed for reconstitution and for current Quality Control concentration!!!**

Reconstitute each Quality Control (HIGH and LOW) with Dilution Buffer just prior to the assay. Let it dissolve at least 15 minutes with occasional gentle shaking (not to foam).

**Reconstituted Quality Controls are ready to use, do not dilute them.**

Stability and storage:

The reconstituted Quality Controls must be used immediately or aliquoted and frozen at -20°C for 3 months. Avoid repeated freeze/thaw cycles.



Note:

Concentration of analyte in Quality Control need not be anyhow associated with normal and/or pathological concentrations in serum or another body fluid. Quality Control serves just for control that the kit works in accordance with PDS and CoA and that ELISA test was carried out properly.

**Wash Solution Conc. (10x)**

Dilute Wash Solution Concentrate (10x) ten-fold in distilled water to prepare a 1x working solution. Example: 100 ml of Wash Solution Concentrate (10x) + 900 ml of distilled water for use of all 96-wells.

Stability and storage:

The diluted Wash Solution is stable 1 month when stored at 2-8°C. Opened Wash Solution Concentrate (10x) is stable 3 months when stored at 2-8°C.

## 10. PREPARATION OF SAMPLES

---

The kit measures ZA2G in serum and plasma (EDTA, citrate, heparin).

Samples should be assayed immediately after collection or should be stored at -20°C. Mix thoroughly thawed samples just prior to the assay and avoid repeated freeze/thaw cycles, which may cause erroneous results. Avoid using hemolyzed or lipemic samples.

Dilute samples 5 000x with Dilution Buffer just prior to the assay in two steps as follows:

**Dilution A (100x):**

Add 5 µl of sample into 495 µl of Dilution Buffer and **mix well** (not to foam). Vortex is recommended.

**Dilution B (50x):**

Add 10 µl of Dilution A into 490 µl of Dilution Buffer to prepare final dilution (5000x) and **mix well** (not to foam). Vortex is recommended.

Stability and storage:

Samples should be stored at -20°, or preferably at -70°C for long-term storage. Avoid repeated freeze/ thaw cycles.

**Do not store the diluted samples.**

See Chapter 13 for stability of serum and plasma samples when stored at 2-8°C, effect of freezing/thawing and effect of sample matrix (serum/plasma) on the concentration of ZA2G.

*Note: It is recommended to use a precision pipette and a careful technique to perform the dilution in order to get precise results.*

Ask for information at [info@biovendor.com](mailto:info@biovendor.com) if assaying cerebrospinal fluid samples.

## 11. ASSAY PROCEDURE

---

1. Pipet **100 µl** of diluted Standards, Quality Controls, Dilution Buffer (=Blank) and samples, preferably in duplicates, into the appropriate wells. See *Figure 1* for example of work sheet.
2. Incubate the plate at room temperature (ca. 25°C) for **1 hour**, shaking at ca. 300 rpm on an orbital microplate shaker.
3. Wash the wells 3-times with Wash Solution (0.35 ml per well). After final wash, invert and tap the plate strongly against paper towel.
4. Add **100 µl** of Conjugate Solution into each well.
5. Incubate the plate at room temperature (ca. 25°C) for **1 hour**, shaking at ca. 300 rpm on an orbital microplate shaker.
6. Wash the wells 3-times with Wash Solution (0.35 ml per well). After final wash, invert and tap the plate strongly against paper towel.
7. Add **100 µl** of Substrate Solution into each well. Avoid exposing the microtiter plate to direct sunlight. Covering the plate with e.g. aluminium foil is recommended.
8. Incubate the plate for **10 minutes** at room temperature. The incubation time may be extended [up to 20 minutes] if the reaction temperature is below than 20°C. Do not shake the plate during the incubation.
9. Stop the colour development by adding **100 µl** of Stop Solution.
10. Determine the absorbance of each well using a microplate reader set to 450 nm, preferably with the reference wavelength set to 630 nm (acceptable range: 550 – 650 nm). Subtract readings at 630 nm (550 - 650 nm) from the readings at 450 nm. **The absorbance should be read within 5 minutes following step 9.**

*Note 1: If some samples and standard/s have absorbances above the upper limit of your microplate reader, perform a second reading at 405 nm. A new standard curve, constructed using the values measured at 405 nm, is used to determine ZA2G concentration of off-scale standards and samples. The readings at 405 nm should not replace the readings for samples that were “in range” at 450 nm.*

*Note 2: Manual washing: Aspirate wells and pipet 0.35 ml Wash Solution into each well. Aspirate wells and repeat twice. After final wash, invert and tap the plate strongly against paper towel. Make certain that Wash Solution has been removed entirely.*

	<b>strip 1+2</b>	<b>strip 3+4</b>	<b>strip 5+6</b>	<b>strip 7+8</b>	<b>strip 9+10</b>	<b>strip 11+12</b>
<b>A</b>	<b>Standard 100</b>	<b>QC LOW</b>	Sample 8	Sample 16	Sample 24	Sample 32
<b>B</b>	<b>Standard 50</b>	Sample 1	Sample 9	Sample 17	Sample 25	Sample 33
<b>C</b>	<b>Standard 25</b>	Sample 2	Sample 10	Sample 18	Sample 26	Sample 34
<b>D</b>	<b>Standard 12</b>	Sample 3	Sample 11	Sample 19	Sample 27	Sample 35
<b>E</b>	<b>Standard 6</b>	Sample 4	Sample 12	Sample 20	Sample 28	Sample 36
<b>F</b>	<b>Standard 3</b>	Sample 5	Sample 13	Sample 21	Sample 29	Sample 37
<b>G</b>	<b>Blank</b>	Sample 6	Sample 14	Sample 22	Sample 30	Sample 38
<b>H</b>	<b>QC HIGH</b>	Sample 7	Sample 15	Sample 23	Sample 31	Sample 39

*Figure 1: Example of a work sheet.*

## 12. CALCULATIONS

Most microplate readers perform automatic calculations of analyte concentration. The standard curve is constructed by plotting the mean absorbance (Y) of Standards against the known concentration (X) of Standards in logarithmic scale, using the four-parameter algorithm. Results are reported as concentration of ZA2G ng/ml in samples.

Alternatively, the logit log function can be used to linearize the standard curve, i.e. logit of the mean absorbance (Y) is plotted against log of the known concentration (X) of Standards.

**The measured concentration of samples calculated from the standard curve must be multiplied by their respective dilution factor, because samples have been diluted prior to the assay, e.g. 13.5 ng/ml (from standard curve) x 5 000 (dilution factor) = 67.5 µg/ml.**

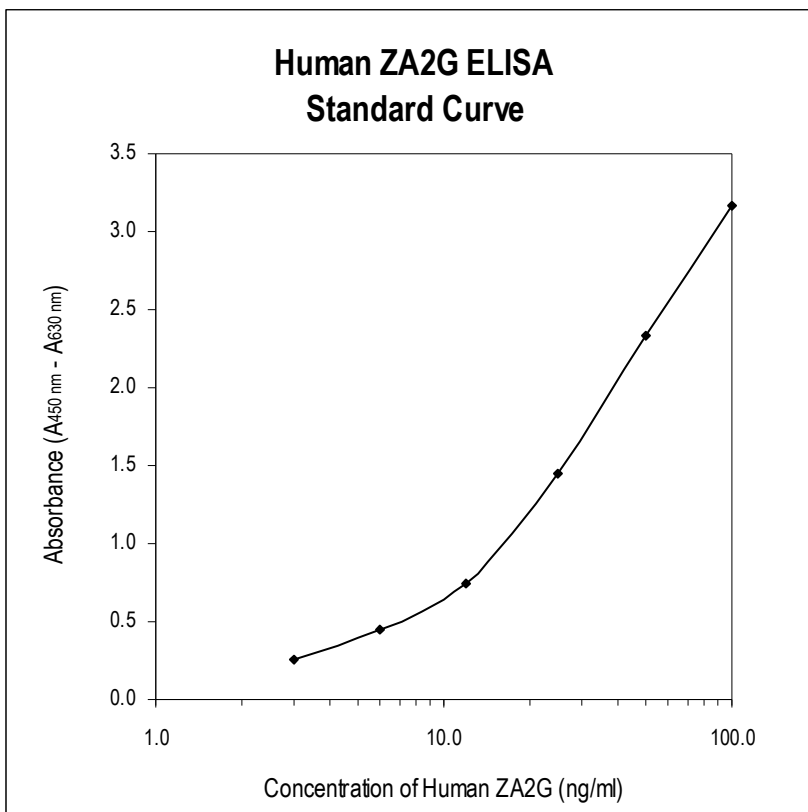


Figure 2: Typical Standard Curve for Human ZA2G ELISA.

## 13. PERFORMANCE CHARACTERISTICS

➤➤ Typical analytical data of BioVendor Human ZA2G ELISA are presented in this chapter

- **Sensitivity**

Limit of Detection (LOD) (defined as concentration of analyte giving absorbance higher than mean absorbance of blank\* plus three standard deviations of the absorbance of blank:  $A_{\text{blank}} + 3 \times \text{SD}_{\text{blank}}$ ) is calculated from the real ZA2G values in wells and is 0.673 ng/ml.

\*Dilution Buffer is pipetted into blank wells.

- **Limit of assay**

Results exceeding ZA2G level of 500 µg/ml should be repeated with more diluted samples. Dilution factor needs to be taken into consideration in calculating the ZA2G concentration.

- **Specificity**

The antibodies used in this ELISA are specific for human ZA2G with no detectable crossreactivities to human leptin, resistin, ANGPTL4, visfatin at 50 ng/ml and human HLA-G at 250 U/ml.

Sera of several mammalian species were measured in the assay. See results below.

For details please contact us at [info@biovendor.com](mailto:info@biovendor.com).

<i>Mammalian serum sample</i>	<i>Observed crossreactivity</i>
Bovine	no
Cat	no
Dog	no
Goat	no
Hamster	no
Horse	no
Monkey	yes
Mouse	no
Pig	no
Rabbit	no
Rat	no
Sheep	no

➤➤ Presented results are multiplied by respective dilution factor

• **Precision**

Intra-assay (Within-Run) (n=8)

Sample	Mean ( $\mu\text{g/ml}$ )	SD ( $\mu\text{g/ml}$ )	CV (%)
1	51.10	1.37	3.0
2	145.00	6.83	4.7

Inter-assay (Run-to-Run) (n=6)

Sample	Mean ( $\mu\text{g/ml}$ )	SD ( $\mu\text{g/ml}$ )	CV (%)
1	192.65	12.45	6.5
2	46.80	3.05	6.6

• **Spiking Recovery**

Serum samples were spiked with different amounts of human ZA2G and assayed.

Sample	Observed ( $\mu\text{g/ml}$ )	Expected ( $\mu\text{g/ml}$ )	Recovery O/E (%)
1	49.40	-	-
	117.51	124.40	94.5
	94.10	99.40	94.7
	71.15	74.40	95.6
2	37.85	-	-
	108.15	112.85	95.8
	84.75	87.85	96.4
	63.15	62.85	100.4

• **Linearity**

Serum samples were serially diluted with Dilution Buffer and assayed.

Sample	Dilution	Observed ( $\mu\text{g/ml}$ )	Expected ( $\mu\text{g/ml}$ )	Recovery O/E (%)
1	-	201.10	-	-
	2x	100.45	100.55	99.9
	4x	51.45	50.30	102.3
	8x	26.70	25.15	106.2
2	-	142.60	-	-
	2x	71.30	71.30	100.0
	4x	36.40	35.65	102.1
	8x	19.45	17.85	109.2

- **Effect of sample matrix**

Citrate, heparin and EDTA plasmas were compared to respective serum samples from the same 10 individuals. Results are shown below:

Volunteer No.	Serum ( $\mu\text{g/ml}$ )	Plasma ( $\mu\text{g/ml}$ )		
		EDTA	Citrate	Heparin
1	50.3	39.8	41.0	49.7
2	27.7	38.0	34.2	63.5
3	45.3	61.1	41.7	50.9
4	50.8	38.8	34.8	41.2
5	46.0	41.9	38.8	43.8
6	43.4	46.8	35.1	31.7
7	35.3	47.3	35.5	35.9
8	30.0	30.1	25.5	32.7
9	25.4	27.5	21.1	30.7
10	42.0	35.8	35.0	34.1
<b>Mean (<math>\mu\text{g/ml}</math>)</b>	<b>39.59</b>	<b>40.69</b>	<b>34.26</b>	<b>41.42</b>
<b>Mean Plasma/Serum (%)</b>	-	<b>102.8</b>	<b>86.5</b>	<b>104.6</b>

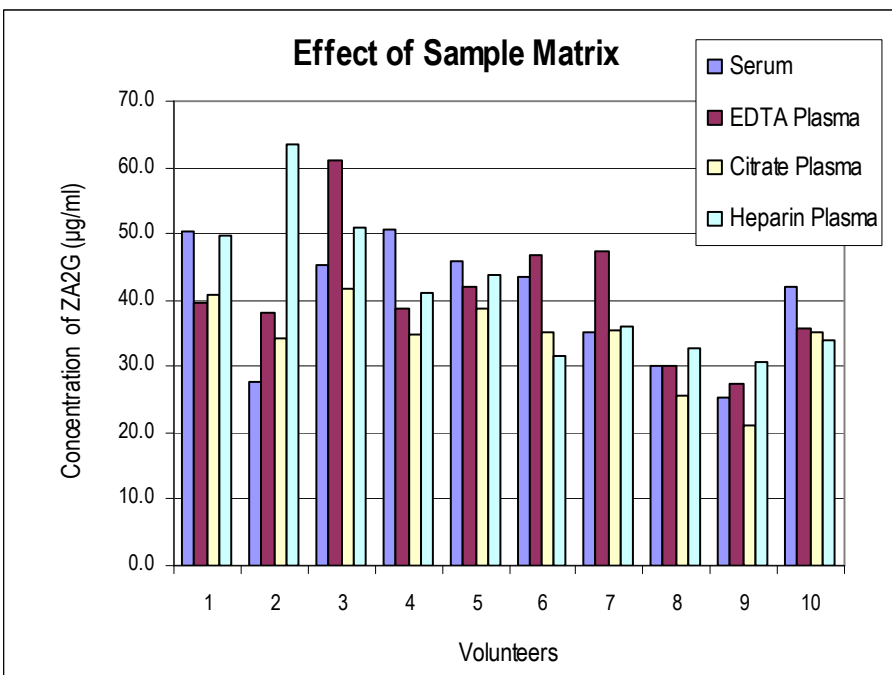


Figure 3: ZA2G levels measured using Human ZA2G ELISA in samples of 10 individuals using serum, EDTA, citrate and heparin plasma, respectively.

- **Stability of samples stored at 2-8°C**

Samples should be stored at -20°C. However, no decline in concentration of ZA2G was observed in serum and plasma samples after 7 days when stored at 2-8°C. To avoid microbial contamination, samples were treated with ε-aminocaproic acid and sodium azide, resulting in the final concentration of 0.03% and 0.1%, respectively.

Sample	Incubation Temp, Period	Serum (µg/ml)	Plasma (µg/ml)		
			EDTA	Citrate	Heparin
1	-20°C	26.75	22.95	19.65	21.60
	2-8°C, 1 day	24.50	22.40	19.55	21.75
	2-8°C, 7 days	25.65	23.40	17.50	23.25
2	-20°C	33.25	28.40	21.40	28.95
	2-8°C, 1 day	27.60	28.85	20.50	27.25
	2-8°C, 7 days	25.80	36.30	20.70	22.80
3	-20°C	35.10	33.70	21.95	26.90
	2-8°C, 1 day	33.90	29.20	24.45	29.75
	2-8°C, 7 days	33.80	30.05	23.10	29.15

- **Effect of Freezing/Thawing**

No decline was observed in concentration of human ZA2G in serum and plasma samples after repeated (5x) freeze/thaw cycles. However it is recommended to avoid unnecessary repeated freezing/thawing of the samples.

Sample	Number of f/t cycles	Serum (µg/ml)	Plasma (µg/ml)		
			EDTA	Citrate	Heparin
1	1x	37.60	34.10	30.30	35.45
	3x	36.56	32.50	30.30	38.35
	5x	36.55	30.80	30.15	34.45
2	1x	30.30	20.80	19.50	26.25
	3x	24.65	23.85	18.45	23.60
	5x	24.85	24.04	21.30	23.15
3	1x	32.90	30.20	23.85	32.65
	3x	37.85	29.20	24.80	29.45
	5x	28.70	30.95	24.10	29.40

- **Reference range**

It is recommended that each laboratory include its own panel of control samples in the assay. Each laboratory should establish its own normal and pathological reference ranges for ZA2G levels with the assay.



## 14. DEFINITION OF THE STANDARD

---

The Standard used in this kit is a recombinant protein produced in 293 cell line (Human embryonic kidney). It is the 41 kDa protein containing 290 AA. The AA sequence (AA 13-290) is identical to Swiss-Prot-P25311(AA 18-295, mature zinc-alpha-2-glycoprotein).

## 15. METHOD COMPARISON

---

BioVendor Human ZA2G ELISA has not been compared to another immunoassay.

## 16. TROUBLESHOOTING AND FAQs

---

### »» Weak signal in all wells

Possible explanations:

- Omission of a reagent or a step
- Improper preparation or storage of a reagent
- Assay performed before reagents were allowed to come to room temperature
- Improper wavelength when reading absorbance

### »» High signal and background in all wells

Possible explanations:

- Improper or inadequate washing
- Overdeveloping; incubation time with Substrate Solution should be decreased before addition of Stop Solution
- Incubation temperature over 30°C

### »» High coefficient of variation (CV)

Possible explanation:

- Improper or inadequate washing
- Improper mixing Standards, Quality Controls or samples

## 17. REFERENCES

---

### »» References to zinc-alpha-2-glycoprotein:

- Araki T, Gejyo F, Takagaki K, Haupt H, Schwick HG, Burgi W, Marti T, Schaller J, Rickli E, Brossmer R, et al.: Complete amino acid sequence of human plasma Zn-alpha 2-glycoprotein and its homology to histocompatibility antigens; *Proc Natl Acad Sci U S A*. 1988 Feb;85(3):679-83.
- Tada T, Ohkubo I, Niwa M, Sasaki M, Tateyama H, Eimoto T.: Immunohistochemical localization of Zn-alpha 2-glycoprotein in normal human tissues; *J Histochem Cytochem*. 1991 Sep;39(9):1221-6.
- Freije JP, Fueyo A, Uria JA, Velasco G, Sanchez LM, Lopez-Boado YS, Lopez-Otin C.: Human Zn-alpha 2-glycoprotein: complete genomic sequence, identification of a related pseudogene and relationship to class I major histocompatibility complex genes; *Genomics*. 1993 Dec;18(3):575-87.
- Lopez-Boado YS, Diez-Itza I, Tolivia J, Lopez-Otin C.: Glucocorticoids and androgens up-regulate the Zn-alpha 2-glycoprotein messenger RNA in human breast cancer cells; *Breast Cancer Res Treat*. 1994;29(3):247-58.
- Sanchez LM, Lopez-Otin C, Bjorkman PJ.: Biochemical characterization and crystalization of human Zn-alpha2-glycoprotein, a soluble class I major histocompatibility complex homolog; *Proc Natl Acad Sci U S A*. 1997 Apr 29;94(9):4626-30.
- Brysk MM, Lei G, Selvanayagam P, Brysk H, Tying SK, Arany I.: Modulation by interferon-gamma of zinc-alpha 2-glycoprotein gene expression in human epithelial cell lines; *Anticancer Res*. 1997 Sep-Oct;17(5A):3387-91.
- Todorov PT, McDevitt TM, Meyer DJ, Ueyama H, Ohkubo I, Tisdale MJ.: Purification and characterization of a tumor lipid-mobilizing factor; *Cancer Res*. 1998 Jun 1;58(11):2353-8.
- Hirai K, Hussey HJ, Barber MD, Price SA, Tisdale MJ.: Biological evaluation of a lipid-mobilizing factor isolated from the urine of cancer patients; *Cancer Res*. 1998 Jun 1;58(11):2359-65.
- Brysk MM, Lei G, Adler-Storthz K, Chen Z, Brysk H, Tying SK, Arany I.: Zinc-alpha2-glycoprotein expression as a marker of differentiation in human oral tumors; *Cancer Lett*. 1999 Mar 22;137(1):117-20.
- Hale LP, Price DT, Sanchez LM, Demark-Wahnefried W, Madden JF.: Zinc alpha-2-glycoprotein is expressed by malignant prostatic epithelium and may serve as a potential serum marker for prostate cancer; *Clin Cancer Res*. 2001 Apr;7(4):846-53.
- Hale LP.: Zinc alpha-2-glycoprotein regulates melanin production by normal and malignant melanocytes; *J Invest Dermatol*. 2002 Aug;119(2):464-70.
- Gohda T, Makita Y, Shike T, Tanimoto M, Funabiki K, Horikoshi S, Tomino Y.: Identification of epistatic interaction involved in obesity using the KK/Ta mouse as a Type 2 diabetes model: is Zn-alpha2 glycoprotein-1 a candidate gene for obesity? *Diabetes*. 2003 Aug;52(8):2175-81.

- Bing C, Bao Y, Jenkins J, Sanders P, Manieri M, Cinti S, Tisdale MJ, Trayhurn P.: Zinc-alpha2-glycoprotein, a lipid mobilizing factor, is expressed in adipocytes and is up-regulated in mice with cancer cachexia; *Proc Natl Acad Sci U S A*. 2004 Feb 24;101(8):2500-5.
- Russell ST, Zimmerman TP, Domin BA, Tisdale MJ.: Induction of lipolysis in vitro and loss of body fat in vivo by zinc-alpha2-glycoprotein; *Biochim Biophys Acta*. 2004 Feb 27;1636(1):59-68.
- Sanders PM, Tisdale MJ.: Effect of zinc-alpha2-glycoprotein (ZAG) on expression of uncoupling proteins in skeletal muscle and adipose tissue; *Cancer Lett*. 2004 Aug 20;212(1):71-81.
- Hansson SF, Puchades M, Blennow K, Sjogren M, Davidsson P.: Validation of a prefractionation method followed by two-dimensional electrophoresis - Applied to cerebrospinal fluid proteins from frontotemporal dementia patients; *Proteome Sci*. 2004 Nov 18;2(1):7.
- Bao Y, Bing C, Hunter L, Jenkins JR, Wabitsch M, Trayhurn P.: Zinc-alpha2-glycoprotein, a lipid mobilizing factor, is expressed and secreted by human (SGBS) adipocytes; *FEBS Lett*. 2005 Jan 3;579(1):41-7.
- Russell ST, Tisdale MJ.: The role of glucocorticoids in the induction of zinc-alpha2-glycoprotein expression in adipose tissue in cancer cachexia; *Br J Cancer*. 2005 Mar 14;92(5):876-81.
- Russell ST, Tisdale MJ.: Effect of eicosapentaenoic acid (EPA) on expression of a lipid mobilizing factor in adipose tissue in cancer cachexia; *Prostaglandins Leukot Essent Fatty Acids*. 2005 Jun;72(6):409-14.
- Jain S, Rajput A, Kumar Y, Uppuluri N, Arvind AS, Tatu U.: Proteomic analysis of urinary protein markers for accurate prediction of diabetic kidney disorder; *J Assoc Physicians India*. 2005 Jun;53:513-20.
- Kamoshida S, Watanabe K, Suzuki M, Mizutani Y, Sakamoto K, Sugimoto Y, Oka T, Fukushima M, Tsutsumi Y.: Expression of cancer cachexia-related factors in human cancer xenografts: an immunohistochemical analysis; *Biomed Res*. 2006 Dec;27(6):275-81.
- Rolli V, Radosavljevic M, Astier V, Macquin C, Castan-Laurell I, Visentin V, Guigne C, Carpenne C, Valet P, Gilfillan S, Bahram S.: Lipolysis is altered in MHC class I zinc-alpha(2)-glycoprotein deficient mice; *FEBS Lett*. 2007 Feb 6;581(3):394-400.









## ➤➤ References to this product:

- Jernas M, Olsson B, Sjöholm K, Sjogren A, Rudemo M, Nellgard B, Carlsson LM, Sjöström CD: Changes in adipose tissue gene expression and plasma levels of adipokines and acute-phase proteins in patients with critical illness. *Metabolism*. 2009 Jan;58 (1):102-8
- Ceperuelo-Mallafre V, Naf S, Escote X, Caubet E, Gomez JM, Miranda M, Chacon MR, Gonzalez-Clemente JM, Gallart L, Gutierrez C, Vendrell J: Circulating and adipose tissue gene expression of zinc-alpha2-glycoprotein in obesity: its relationship with adipokine and lipolytic gene markers in subcutaneous and visceral fat. *J Clin Endocrinol Metab*. 2009 Dec;94 (12):5062-9


- Stejskal D, Karpísek M, Reutová H, Stejskal P, Kotolová H, Kollár P: Determination of serum zinc-alpha-2-glycoprotein in patients with metabolic syndrome by a new ELISA. *Clin Biochem.* 2008 Mar;41(4-5):313-6
- Ding Q, Mracek T, Gonzalez-Muniesa P, Kos K, Wilding J, Trayhurn P, Bing C: Identification of macrophage inhibitory cytokine-1 in adipose tissue and its secretion as an adipokine by human adipocytes. *Endocrinology.* 2009 Apr;150 (4):1688-96
- Selva DM, Lecube A, Hernandez C, Baena JA, Fort JM, Simo R: Lower zinc-alpha2-glycoprotein production by adipose tissue and liver in obese patients unrelated to insulin resistance. *J Clin Endocrinol Metab.* 2009 Nov;94 (11):4499-507
- Brettschneider J, Mogel H, Lehmsiek V, Ahlert T, Sussmuth S, Ludolph AC, Tumani H: Proteome Analysis of Cerebrospinal Fluid in Amyotrophic Lateral Sclerosis (ALS). *Neurochem Res.* 2008 May 15;
- Roher AE, Maarouf CL, Sue LI, Hu Y, Wilson J, Beach TG: Proteomics-derived cerebrospinal fluid markers of autopsy-confirmed Alzheimer's disease. *Biomarkers.* 2009 Nov;14 (7):493-501
- Fain JN, Taguele BM, Cheema P, Madan AK, Tichansky DS: Release of 12 Adipokines by Adipose Tissue, Nonfat Cells, and Fat Cells From Obese Women. *Obesity (Silver Spring).* 2009 Oct 15;
- Yeung DC, Lam KS, Wang Y, Tso AW, Xu A: Serum zinc-alpha2-glycoprotein correlates with adiposity, triglycerides, and the key components of the metabolic syndrome in chinese subjects. *J Clin Endocrinol Metab.* 2009 Jul;94 (7):2531-6

➤➤ For more references on this product see our WebPages at [www.biovendor.com](http://www.biovendor.com)

## 18. EXPLANATION OF SYMBOLS

	Catalogue number
	Content
	Lot number
	See instructions for use
	Biological hazard
	Expiry date
	Storage conditions
	Identification of packaging materials


# Assay Procedure Summary

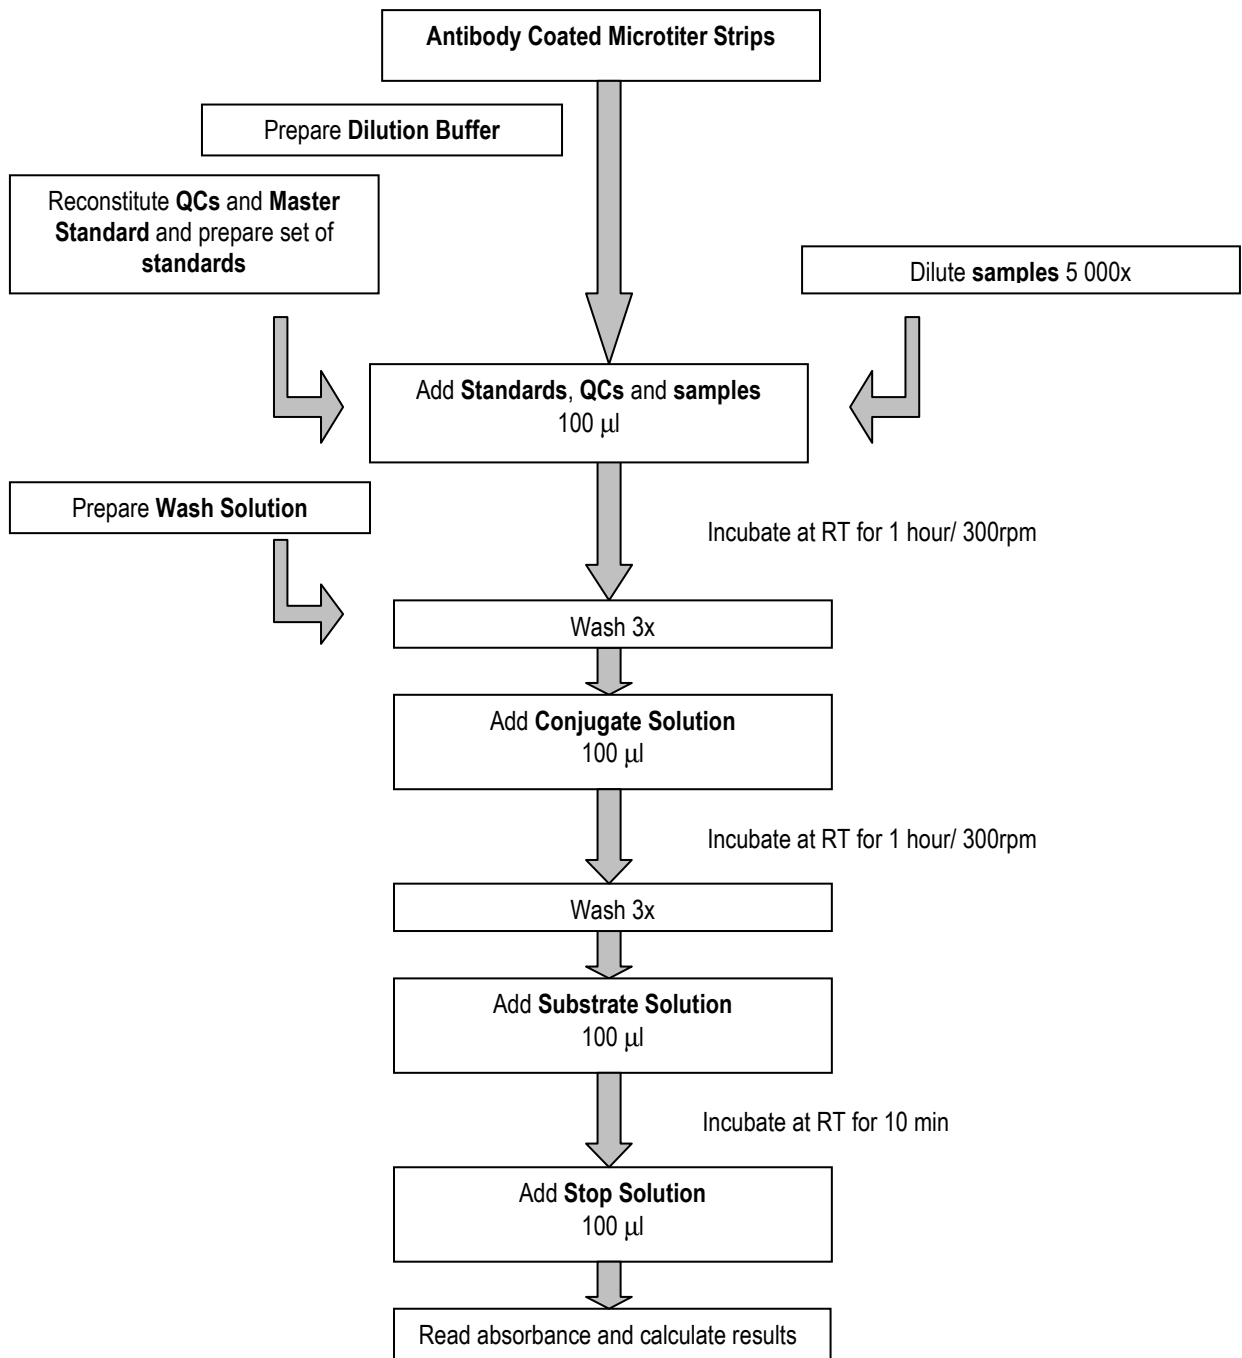

12								
11								
10								
9								
8								
7								
6								
5								
4								
3								
2								
1								
	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>

# BioVendor

Research  
and Diagnostic Products

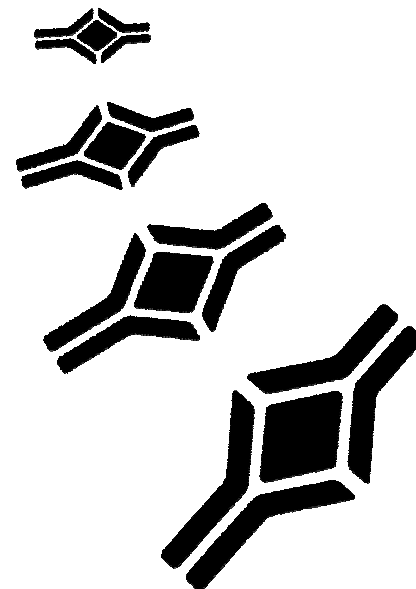

## HEADQUARTERS:

BioVendor - Laboratorní  
medicína a.s.

Karasek 1767/1

621 00 Brno  
CZECH REPUBLIC

Phone: +420-549-124-185  
Fax: +420-549-211-460

E-mail: [info@biovendor.com](mailto:info@biovendor.com)  
[sales@biovendor.com](mailto:sales@biovendor.com)  
Web: [www.biovendor.com](http://www.biovendor.com)

EUROPEAN UNION:  
BioVendor GmbH

Im Neuenheimer Feld 583

D-69120 Heidelberg  
GERMANY

Phone: +49-6221-433-9100  
Fax: +49-6221-433-9111

E-mail: [infoEU@biovendor.com](mailto:infoEU@biovendor.com)

USA, CANADA AND MEXICO:  
BioVendor LLC

128 Bingham Rd.  
Suite 1300

Asheville, NC 28806  
USA

Phone: +1-828-575-9250  
+1-800-404-7807  
Fax: +1-828-575-9251

E-mail: [infoUSA@biovendor.com](mailto:infoUSA@biovendor.com)

CHINA - Hong Kong Office:  
BioVendor Laboratories Ltd

Room 4008  
Hong Kong Plaza, No.188

Connaught Road West  
Hong Kong, CHINA

Phone: +852-2803-0523  
Fax: +852-2803-0525

E-mail: [infoHK@biovendor.com](mailto:infoHK@biovendor.com)

CHINA – Mainland Office:  
BioVendor Laboratories Ltd

Room 2917, 29/F  
R & F Ying Feng Plaza, No.2  
Huaqiang road

Pearl River New Town  
Guang Zhou, CHINA

Phone: +86-20-38065519  
Fax: +86-20-38065529

E-mail: [infoCN@biovendor.com](mailto:infoCN@biovendor.com)