


BioVendor

Research
and Diagnostic Products

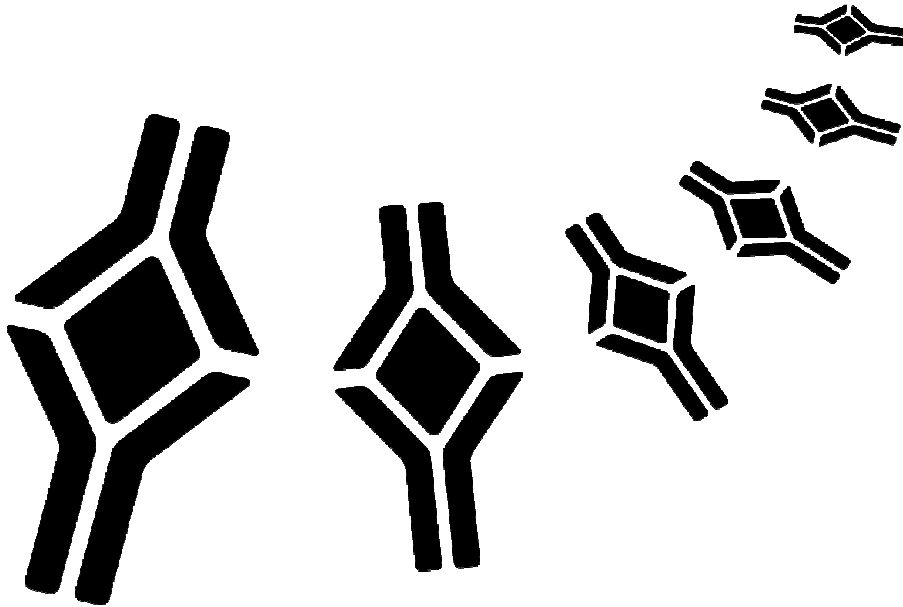

HUMAN CYSTATIN C ELISA

Product Data Sheet

Cat. No.: RD191009100

European
Union:



Rest of the world:
For research use only!

CONTENTS

1.	INTENDED USE	3
2.	STORAGE, EXPIRATION	3
3.	INTRODUCTION	4
4.	TEST PRINCIPLE	5
5.	PRECAUTIONS	5
6.	TECHNICAL HINTS	6
7.	REAGENT SUPPLIED	6
8.	MATERIAL REQUIRED BUT NOT SUPPLIED	7
9.	PREPARATION OF REAGENTS	7
10.	PREPARATION OF SAMPLES	10
11.	ASSAY PROCEDURE	11
12.	CALCULATIONS	13
13.	PERFORMANCE CHARACTERISTICS	14
14.	DEFINITION OF THE STANDARD	19
15.	URINE CYSTATIN C DETERMINATION	19
16.	PRELIMINARY POPULATION AND CLINICAL DATA	21
17.	METHOD COMPARISON	23
18.	TROUBLESHOOTING AND FAQs	24
19.	REFERENCES	25
20.	EXPLANATION OF SYMBOLS	28

**»» This kit is manufactured by:
BioVendor – Laboratorní medicína a.s.**

»» Use only the current version of Product Data Sheet enclosed with the kit!

1. INTENDED USE

The RD191009100 Human Cystatin C ELISA is a sandwich enzyme immunoassay for the quantitative measurement of human cystatin C.

»» Features

- **European Union: for *in vitro* diagnostic use**
Rest of the world: for research use only!
- The total assay time is less than 2 hours
- The kit measures total cystatin C in serum, plasma (EDTA, citrate, heparin), urine and cerebrospinal fluid
- Assay format is 96 wells
- Quality Controls are human serum or human urine native protein based. No animal sera are used
- Standard is purified native protein based
- Components of the kit are provided ready to use or concentrated
- Convenient for automatization

2. STORAGE, EXPIRATION

Store the complete kit at 2-8°C. Under these conditions, the kit is stable until the expiration date (see label on the box).

For stability of opened reagents see Chapter 9.

3. INTRODUCTION

Cysteine proteinase inhibitors, cystatins superfamily, have been identified in animals, plants and protozoa. All cystatins inactivate lysosomal cysteine proteinases, e.g. cathepsin B, H, K, L and S as well as some structurally related plant proteinases, such as papain and actinidin. Human cystatin C is produced at a constant rate by all nucleated body cells and occurs in all body fluids abundantly. It is a non-glycosylated basic single-chain protein consisting of 120 amino acids with a molecular weight of 13.36 kDa and is characterized by two disulfide bonds in the carboxy-terminal region. The protein is encoded by the CS73 gene located on the short arm of chromosome 20.

Biological function of human cystatin C, and its role in various pathological states, has been the subject of numerous studies. Imbalance between cystatin C and cysteine proteinases is associated with diseases such as inflammation, renal failure, cancer, Alzheimer disease, multiple sclerosis and hereditary cystatin C amyloid angiopathy. Its increased level has been found in patients with autoimmune diseases, with colorectal tumors and metastases, patients with inflammation and in patients on dialysis. Serum cystatin C concentration correlates negatively with glomerular filtration rate (GFR) as well as or better than creatinine, therefore was recently proposed as a new, very sensitive, marker of changes in GFR.

On the other hand, low levels of cystatin C come along the breakdown of the elastic laminae and, subsequently, the atherosclerosis and abdominal aortic aneurysm, as indicate latest publications. Results make evident association of cystatin C levels with the incidence of myocardial infarction, coronary death and angina pectoris. Furthermore, cystatin C correlates with triglycerides, LDL-cholesterol, BMI and age of individuals. Thus, low concentration of cystatin C presents a risk factor for secondary cardiovascular events.

Areas of investigation:

Renal disease

4. TEST PRINCIPLE

In the BioVendor Human Cystatin C ELISA, standards, quality controls and samples are incubated in microtiter plate wells pre-coated with polyclonal anti-human cystatin C antibody. After 30 minutes incubation and washing, polyclonal anti-human cystatin C antibody, conjugated with horseradish peroxidase (HRP) is added to the wells and incubated for 30 minutes with captured cystatin C. Following another washing step, the remaining HRP conjugate is allowed to react with the substrate solution (TMB). The reaction is stopped by addition of acidic solution and absorbance of the resulting yellow product is measured. The absorbance is proportional to the concentration of cystatin C. A standard curve is constructed by plotting absorbance values against concentrations of cystatin C standards, and concentrations of unknown samples are determined using this standard curve.

5. PRECAUTIONS

- **For professional use only**
- Wear gloves and laboratory coats when handling immunodiagnostic materials
- Do not drink, eat or smoke in the areas where immunodiagnostic materials are being handled
- This kit contains components of human origin. These materials were found non-reactive for HBsAg, HCV antibody and for HIV 1/2 antigen and antibody. However, these materials should be handled as potentially infectious, as no test can guarantee the complete absence of infectious agents
- Avoid contact with the acidic Stop Solution and Substrate Solution, which contains hydrogen peroxide and tetramethylbenzidine (TMB). Wear gloves and eye and clothing protection when handling these reagents. Stop and/or Substrate Solutions may cause skin/eyes irritation. In case of contact with the Stop Solution and the Substrate Solution wash skin/eyes thoroughly with water and seek medical attention, when necessary
- The materials must not be pipetted by mouth

6. TECHNICAL HINTS

- Reagents with different lot numbers should not be mixed
- Use thoroughly clean glassware
- Use deionized (distilled) water, stored in clean containers
- Avoid any contamination among samples and reagents. For this purpose, disposable tips should be used for each sample and reagent
- Substrate Solution should remain colourless until added to the plate. Keep Substrate Solution protected from light
- Stop Solution should remain colourless until added to the plate. The colour developed in the wells will turn from blue to yellow immediately after the addition of the Stop Solution. Wells that are green in colour indicate that the Stop Solution has not mixed thoroughly with the Substrate Solution
- Dispose of consumable materials and unused contents in accordance with applicable national regulatory requirements

7. REAGENT SUPPLIED

<i>Kit Components</i>	<i>State</i>	<i>Quantity</i>
Antibody Coated Microtiter Strips	ready to use	96 wells
Conjugate Solution Conc. (50x)	concentrated	0.26 ml
Conjugate Diluent	ready to use	13 ml
Set of Standards	concentrated	6 x 0.1 ml
Quality Control HIGH	concentrated	0.1 ml
Quality Control LOW	concentrated	0.1 ml
Dilution Buffer Conc. (10x)	concentrated	10 ml
Wash Solution Conc. (10x)	concentrated	100 ml
Substrate Solution	ready to use	13 ml
Stop Solution	ready to use	13 ml
Product Data Sheet + Certificate of Analysis	-	1 pc

8. MATERIAL REQUIRED BUT NOT SUPPLIED

- Deionized (distilled) water
- Test tubes for diluting samples
- Glassware (graduated cylinder and bottle) for Wash Solution (Dilution Buffer)
- Precision pipettes to deliver 10-1000 μ l with disposable tips
- Multichannel pipette to deliver 100 μ l with disposable tips
- Absorbent material (e.g. paper towels) for blotting the microtiter plate after washing
- Vortex mixer
- Orbital microplate shaker capable of approximately 300 rpm
- Microplate washer (optional). [Manual washing is possible but not preferable.]
- Microplate reader with 450 ± 10 nm filter, preferably with reference wavelength 630 nm (alternatively another one from the interval 550-650 nm)
- Software package facilitating data generation and analysis (optional)

9. PREPARATION OF REAGENTS

- All reagents need to be brought to room temperature prior to use
- Always prepare only the appropriate quantity of reagents for your test
- Do not use components after the expiration date marked on their label

- Assay reagents supplied ready to use:

Antibody Coated Microtiter Strips

Stability and storage:

Return the unused strips to the provided aluminium zip-sealed bag with desiccant and seal carefully. Remaining Microtiter Strips are stable 3 months stored at 2-8°C and protected from the moisture.

Conjugate Diluent

Substrate Solution

Stop Solution

Stability and storage:

Opened reagents are stable 3 months when stored at 2-8°C.

- **Assay reagents supplied concentrated:**

Dilution Buffer Conc. (10x)

Dilute Dilution Buffer Concentrate (10x) ten-fold in 90 ml distilled water to prepare a 1x working solution, e.g. 10 ml of Dilution Buffer Concentrate (10x) + 90 ml of distilled water for use of all 96-wells.

It is recommended to dilute only such a volume of Dilution Buffer Concentrate (10x) to be used up in the one run of the test.

Stability and storage:

The diluted Dilution Buffer is stable 1 week when stored at 2-8°C. Opened Dilution Buffer Concentrate (10x) is stable 3 months when stored at 2-8°C.

Set of Standards

Dilute each concentration of Standard 400x with the Dilution Buffer just prior to the assay in two steps as follows:

Dilution A (10x):

Add 10 µl of Standard into 90 µl of Dilution Buffer. **Mix well** (not to foam). Vortex is recommended.

Dilution B (40x):

Add 10 µl of Dilution A into 390 µl of Dilution Buffer to prepare final dilution (400x). **Mix well** (not to foam). Vortex is recommended.

Stability and storage:

Opened Standards are stable 3 months when stored at 2-8°C.

Do not store the diluted Set of Standards.

Quality Controls HIGH, LOW

Refer to the Certificate of Analysis for current Quality Control concentration!!!

Dilute each Quality Control (QC) 400x with the Dilution Buffer just prior to the assay in two steps as follows:

Dilution A (10x):

Add 10 µl of QC into 90 µl of Dilution Buffer. **Mix well** (not to foam). Vortex is recommended.

Dilution B (40x):

Add 10 µl of Dilution A into 390 µl of Dilution Buffer to prepare final dilution (400x). **Mix well** (not to foam). Vortex is recommended.

Stability and storage:

Opened Quality Controls are stable 3 months when stored at 2-8°C.

Do not store the diluted Quality Controls.

Note:

Concentration of analyte in Quality Controls need not be anyhow associated with normal and/or pathological concentrations in serum or another body fluid. Quality Controls serve just for control that the kit works in accordance with PDS and CoA and that ELISA test was carried out properly.

It is recommended to supplement two or three negative sample controls of customer's own (in addition to those provided with this kit). They can serve as evidence of the difference between positive and negative samples (see *Figure 5* and *Figure 6*).

Conjugate Solution Conc. (50x)

Prepare the working Conjugate Solution by adding 1 part Conjugate Solution Concentrate (50x) with 49 parts Conjugate Diluent.

Example: 0.25 ml of Conjugate Solution Concentrate (50x) + 12.25 ml of Conjugate Diluent for use of all 96-wells. Prepare only the volume needed for the test. **Mix well** (not to foam).

Stability and storage:

Opened Conjugate Solution Concentrate (50x) is stable 3 months when stored at 2-8°C.

Do not store the diluted Conjugate Solution.

Wash Solution Conc. (10x)

Dilute Wash Solution Concentrate (10x) ten-fold in 900 ml of distilled water to prepare a 1x working solution, e.g. 100 ml of Wash Solution Concentrate (10x) + 900 ml of distilled water for use of all 96-wells.

Stability and storage:

The diluted Wash Solution is stable 1 month when stored at 2-8°C. Opened Wash Solution Concentrate (10x) is stable 3 months when stored at 2-8°C.

10. PREPARATION OF SAMPLES

The kit measures cystatin C in serum, plasma (EDTA, citrate, heparin), urine and cerebrospinal fluid.

Samples should be assayed immediately after collection or should be stored at -20°C. Mix thoroughly thawed samples just prior to the assay and avoid repeated freeze/thaw cycles, which may cause erroneous results. Avoid using hemolyzed or lipemic samples.

Dilute samples (serum, plasma) 400x with the Dilution Buffer just prior to the assay in two steps as follows:

Dilution A (10x):

Add 10 µl of sample into 90 µl of Dilution Buffer. **Mix well** (not to foam). Vortex is recommended.

Dilution B (40x):

Add 10 µl of Dilution A into 390 µl of Dilution Buffer to prepare final dilution (400x). **Mix well** (not to foam). Vortex is recommended.

Dilute samples (CSF) 1 600x with the Dilution Buffer just prior to the assay as follows:

Dilution A (40x):

Add 10 µl of sample into 390 µl of Dilution Buffer. **Mix well** (not to foam). Vortex is recommended.

Dilution B (40x):

Add 10 µl of Dilution A into 390 µl of Dilution Buffer to prepare final dilution (1 600x). **Mix well** (not to foam). Vortex is recommended.

Stability and storage:

Samples should be stored at -20°, or preferably at -70°C for long-term storage. Avoid repeated freeze/ thaw cycles.

Do not store the diluted samples.

For dilution of urine samples see Chapter 15.

See Chapter 13 for stability of serum and plasma samples when stored at 2-8°C, effect of freezing/thawing and effect of sample matrix (serum/plasma) on the concentration of cystatin C.

Note: It is recommended to use a precision pipette and a careful technique to perform the dilution in order to get precise results.

11. ASSAY PROCEDURE

1. Pipet **100 µl** of diluted Standards, Quality Controls, Dilution Buffer (=Blank) and samples, preferably in duplicates, into the appropriate wells. See *Figure 1* for example of work sheet.
2. Incubate the plate at room temperature (ca. 25°C) for **30 minutes**, shaking at ca. 300 rpm on an orbital microplate shaker.
3. Wash the wells 3-times with Wash Solution (0.35 ml per well). After final wash, invert and tap the plate strongly against paper towel.
4. Add **100 µl** of Conjugate Solution into each well.
5. Incubate the plate at room temperature (ca. 25°C) for **30 minutes**, shaking at ca. 300 rpm on an orbital microplate shaker. Incubation without shaking is an alternative that requires extended incubation with substrate – see step 8 below.
6. Wash the wells 3-times with Wash Solution (0.35 ml per well). After final wash, invert and tap the plate strongly against paper towel.
7. Add **100 µl** of Substrate Solution into each well. Avoid exposing the microtiter plate to direct sunlight. Covering the plate with e.g. aluminium foil is recommended.
8. Incubate the plate for **10 minutes** at room temperature. The incubation time may be extended [up to 20 minutes] if the reaction temperature is below than 20°C. Do not shake with the plate during the incubation.
9. Stop the colour development by adding **100 µl** of Stop Solution.
10. Determine the absorbance of each well using a microplate reader set to 450 nm, preferably with the reference wavelength set to 630 nm (acceptable range: 550 - 650 nm). Subtract readings at 630 nm (550 - 650 nm) from the readings at 450 nm.
The absorbance should be read within 5 minutes following step 9.

Note: If some samples and standard/s have absorbances above the upper limit of your microplate reader, perform a second reading at 405 nm. A new standard curve, constructed using the values measured at 405 nm, is used to determine cystatin C concentration of off-scale standards and samples. The readings at 405 nm should not replace the readings for samples that were “in range” at 450 nm.

Note 2: Manual washing: Aspirate wells and pipet 0.35 ml Wash Solution into each well. Aspirate wells and repeat twice. After final wash, invert and tap the plate strongly against paper towel. Make certain that Wash Solution has been removed entirely.

	strip 1+2	strip 3+4	strip 5+6	strip 7+8	strip 9+10	strip 11+12
A	Standard 10 000	Blank	Sample 8	Sample 16	Sample 24	Sample 32
B	Standard 4 000	Sample 1	Sample 9	Sample 17	Sample 25	Sample 33
C	Standard 2 000	Sample 2	Sample 10	Sample 18	Sample 26	Sample 34
D	Standard 1 000	Sample 3	Sample 11	Sample 19	Sample 27	Sample 35
E	Standard 400	Sample 4	Sample 12	Sample 20	Sample 28	Sample 36
F	Standard 200	Sample 5	Sample 13	Sample 21	Sample 29	Sample 37
G	QC HIGH	Sample 6	Sample 14	Sample 22	Sample 30	Sample 38
H	QC LOW	Sample 7	Sample 15	Sample 23	Sample 31	Sample 39

Figure 1: Example of a work sheet.

12. CALCULATIONS

Most microplate readers perform automatic calculations of analyte concentration. The Standard curve is constructed by plotting the mean absorbance (Y) of Standards against the known concentration (X) of Standards in logarithmic scale, using the four-parameter algorithm. Results are reported as concentration of cystatin C ng/ml in samples.

Alternatively, the *logit log* function can be used to linearize the standard curve, i.e. *logit* of the mean absorbance (Y) is plotted against *log* of the known concentration (X) of Standards. Use values of undiluted standard range: 10 000, 4 000, 2 000, 1 000, 400, 200 ng/ml.

Samples, Quality Controls and Standards are all diluted 400x prior to analysis, so there is no need to take this dilution factor into account.

Results are reported as total concentration of cystatin C (ng/ml) in serum/plasma samples. For the determination of concentration in samples diluted differently, use dilution factor for dividing/multiplying results read off the standard curve.

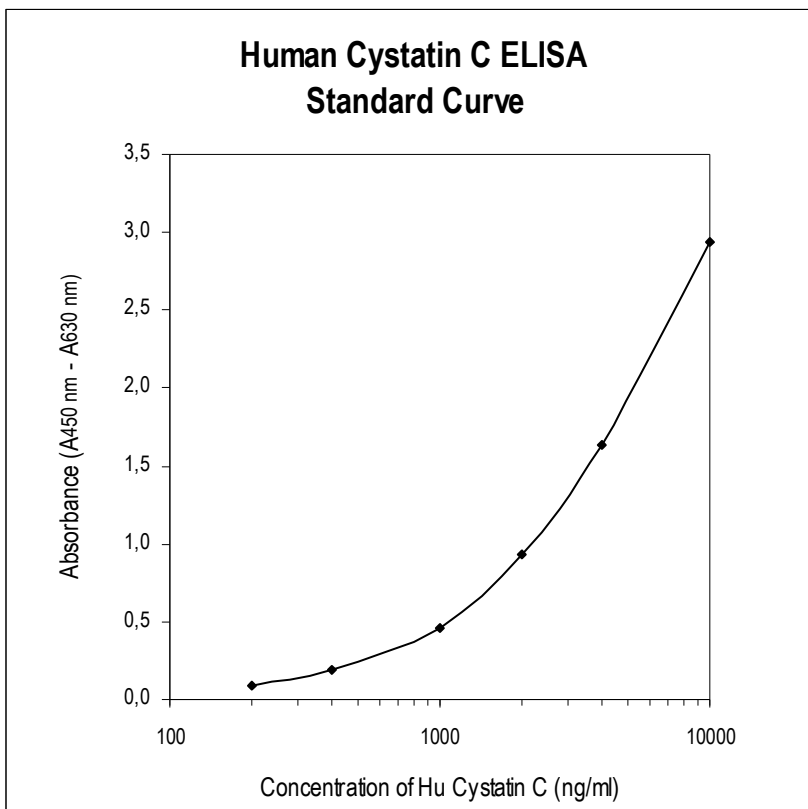


Figure 2: Typical Standard Curve for Human Cystatin C ELISA.

13. PERFORMANCE CHARACTERISTICS

➤➤ **Typical analytical data of BioVendor Human Cystatin C ELISA are presented in this chapter**

- **Sensitivity**

Limit of Detection (LOD) (defined as concentration of analyte giving absorbance higher than mean absorbance of blank* plus three standard deviations of the absorbance of blank: $A_{\text{blank}} + 3 \times \text{SD}_{\text{blank}}$) is calculated from the real cystatin C values in wells and is 0.25 ng/ml.

*Dilution Buffer is pipetted into blank wells.

- **Limit of assay**

Results exceeding cystatin C level of 10 000 ng/ml should be repeated with more diluted samples. Dilution factor needs to be taken into consideration in calculating the cystatin C concentration.

Example: Dilute samples **800x** and dilution factor needs to be taken into consideration. The result (read off standard curve) is then **multiplied by 2**.

Conversely: If sample is diluted only **50x** instead of **400x**, due to lower concentration of analyte, the result (read off the standard curve) is **divided by** dilution factor **8**, in this case.

Standard curve is plotted without changes, in both above mentioned cases, i.e. in undiluted concentrations: 10 000, 4 000, 2 000, 1 000, 400 and 200 ng/ml.

Note: cystatin C standard range 10 000-200 ng/ml, after 400x dilution, results in the actual concentration range 25-0.25 ng/ml, which represents concentration 2.5-0.025 ng/well.

Thus, the assay system is capable of measuring these concentrations 25-0.25 ng/ml in 400x diluted samples, which can help to decide what dilution choose for samples other than sera.

- **Specificity**

The antibodies used in this ELISA are specific for human cystatin C.

Determination of cystatin C does not interfere with hemoglobin (1.0 mg/ml), bilirubin (170 $\mu\text{mol/l}$) and triglycerides (5.0 mmol/l).

Sera of several mammalian species were measured in the assay. See results below.

For details please contact us at info@biovendor.com.

<i>Mammalian serum sample</i>	<i>Observed crossreactivity</i>
Bovine	no
Cat	no
Dog	no
Goat	no
Hamster	no
Horse	no
Monkey	yes
Mouse	no
Pig	no
Rabbit	no
Rat	no
Sheep	no

- **Precision**

Intra-assay (Within-Run) (n=8)

<i>Sample</i>	<i>Mean (ng/ml)</i>	<i>SD (ng/ml)</i>	<i>CV (%)</i>
1	1 544	154	3.1
2	1 790	172	1.9

Inter-assay (Run-to-Run) (n=5)

<i>Sample</i>	<i>Mean (ng/ml)</i>	<i>SD (ng/ml)</i>	<i>CV (%)</i>
1	1 440	49	3.4
2	1 712	179	10.4

- **Spiking Recovery**

Serum samples were spiked with different amounts of human cystatin C, diluted with Dilution Buffer 400x and assayed.

<i>Sample</i>	<i>Observed (ng/ml)</i>	<i>Expected (ng/ml)</i>	<i>Recovery O/E (%)</i>
1	771	-	-
	1 146	1 171	98
	1 435	1 571	91
	2 702	2 771	98
2	978	-	-
	1 338	1 378	97
	1 566	1 778	88
	2 904	2 978	98

- **Linearity**

Serum samples were serially diluted with Dilution Buffer after primary dilution 400x and assayed.

<i>Sample</i>	<i>Dilution</i>	<i>Observed (ng/ml)</i>	<i>Expected (ng/ml)</i>	<i>Recovery O/E (%)</i>
1	-	2 773	-	-
	2x	1 340	1 387	97
	4x	662	693	95
	8x	353	347	102
2	-	2 682	-	-
	2x	1 289	1 341	96
	4x	656	671	98
	8x	331	335	99

- **Effect of sample matrix**

EDTA, citrate and heparin plasmas were compared to respective serum samples from the same 10 individuals.

Results are shown below:

Volunteer No.	Serum (ng/ml)	Plasma (ng/ml)		
		EDTA	Citrate	Heparin
1	759	744	647	903
2	763	755	749	885
3	623	610	499	829
4	491	465	444	543
5	625	707	679	815
6	1 206	737	712	862
7	676	706	574	753
8	619	646	624	690
9	605	669	668	570
10	527	631	528	619
Mean (ng/ml)	689	667	612	747
Mean Plasma/Serum (%)		97%	89%	108%
Coefficient of determination R²		0.97	0.97	0.97

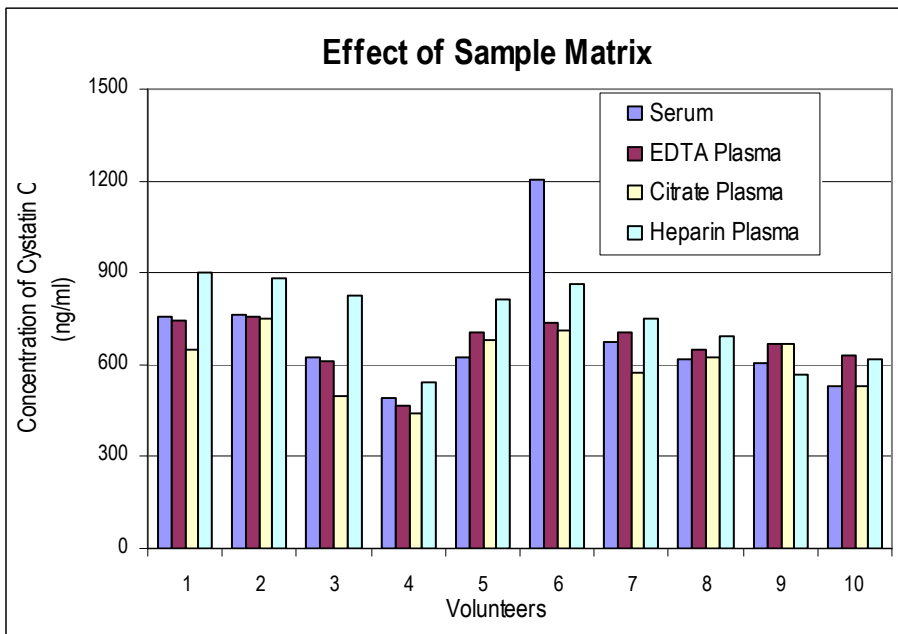


Figure 3: Cystatin C levels measured using Human Cystatin C ELISA from 10 individuals using serum, EDTA, citrate and heparin plasma, respectively.

- **Stability of samples stored at 2-8°C**

Samples should be stored at -80°C. However, no decline in concentration of cystatin C was observed in serum and plasma samples after 7 days when stored at 2-8°C. To avoid microbial contamination, samples were treated with ε-aminocaproic acid and sodium azide, resulting in the final concentration of 0.03% and 0.1%, respectively.

Sample	Incubation Temp, Period	Serum (ng/ml)	Plasma (ng/ml)		
			EDTA	Citrate	Heparin
1	-80°C	1 023	700	620	639
	2-8°C, 1 day	921	773	592	648
	2-8°C, 7 day	1 171	762	615	647
2	-80°C	707	719	571	621
	2-8°C, 1 day	725	737	568	606
	2-8°C, 7 day	618	634	482	563
3	-80°C	625	660	483	603
	2-8°C, 1 day	639	637	499	620
	2-8°C, 7 day	636	651	552	603
4	-80°C	530	549	466	579
	2-8°C, 1 day	561	568	518	529
	2-8°C, 7 day	502	610	486	512

- **Effect of Freezing/Thawing**

No decline was observed in concentration of human cystatin C in serum and plasma samples after repeated (5x) freeze/thaw cycles. However it is recommended to avoid unnecessary repeated freezing/thawing of the samples.

Sample	Number of f/t cycles	Serum (ng/ml)	Plasma (ng/ml)		
			EDTA	Citrate	Heparin
1	1x	785	774	544	867
	3x	855	765	602	783
	5x	789	755	615	746
2	1x	599	721	613	719
	3x	549	715	531	734
	5x	632	676	632	740
3	1x	618	473	310	624
	3x	523	554	260	545
	5x	593	553	855	629
4	1x	387	518	394	454
	3x	370	411	354	442
	5x	461	465	349	497

14. DEFINITION OF THE STANDARD

The Standard used in this kit is purified native protein based.

15. URINE CYSTATIN C DETERMINATION

For the determination of cystatin C in urine use the serum/plasma protocol only with the following modifications:

- **Sample collection and storage**

It is recommended to freeze down untreated urine although no significant decline was observed in concentration of human cystatin C in samples stored at 4°C for 14 days.

- **Sample preparation**

Dilute urine samples **20x** with Dilution Buffer just prior to use in the assay, e.g.: 20 µl of sample + 380 µl of Dilution Buffer.

Stability and storage:

Untreated urine samples are stable for 3 months when stored at -20°C/ -70°C.

Do not store the diluted samples.

- **Calculations of results**

Standard curve is plotted using values of undiluted Standards: 10 000, 4 000, 2 000, 1 000, 400 and 200 ng/ml. As urine samples are diluted only **20x** whereas Standards are diluted **400x**, the result (read off the Standard curve) has to be divided by **dilution factor 20** in order to obtain the real concentration in the original (undiluted) sample.

- **Effect of freezing/thawing on the concentration of cystatin C in urine**

Cystatin C levels were determined in the morning urine from fifteen individuals who were examined because of a suspicion of renal dysfunction. All of them had urine protein < 0.3 g/day and a normal count of leukocytes in urine.

Assay results are shown below:

Sample No.	Cystatin C (ng/ml)	
	1x F/T	5x F/T
1	31	33
2	62	66
3	30	22
4	11	13
5	24	24
6	22	24
7	48	42
8	32	30
9	27	32
10	101	95
11	39	41
12	51	63
13	10	8
14	84	86
15	47	43

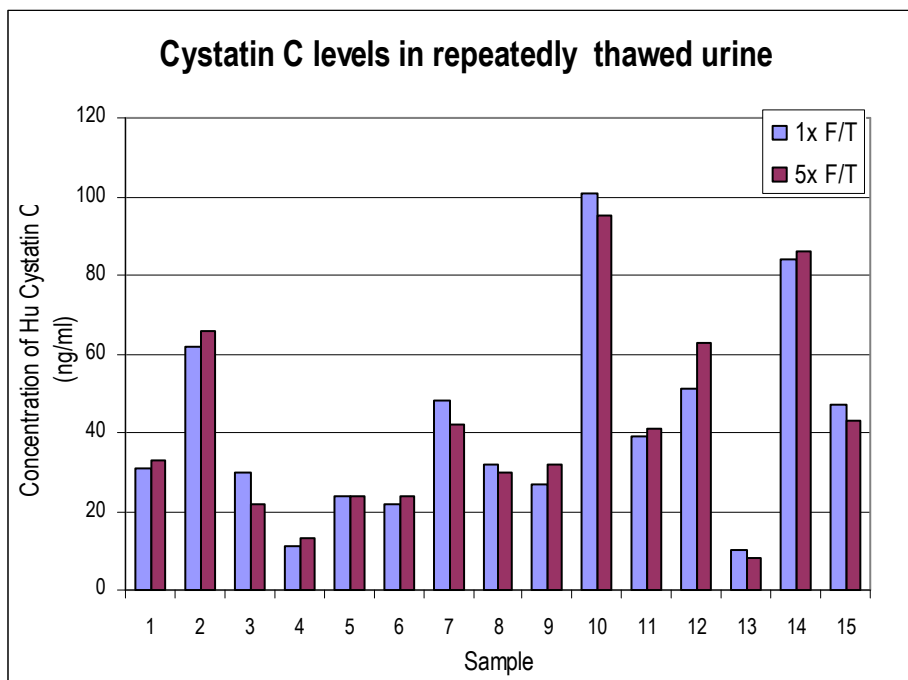


Figure 4: Cystatin C concentration was determined in urine after repeated freeze-thaw cycles. Samples were taken from fifteen individuals who were suspected to have renal dysfunction.

16. PRELIMINARY POPULATION AND CLINICAL DATA

- **Serum cystatin C determination**

Sera from eight patients on long-term dialysis were measured and their cystatin C levels compared to control sera from ten normal, apparently healthy individuals:

Sample No.	Cystatin C (ng/ml)	CV (%)
1	8 335	6
2	8 014	8
3	6 822	1
4	9 464	8
5	7 844	8
6	3 366	4
7	5 955	1
8	3 583	14

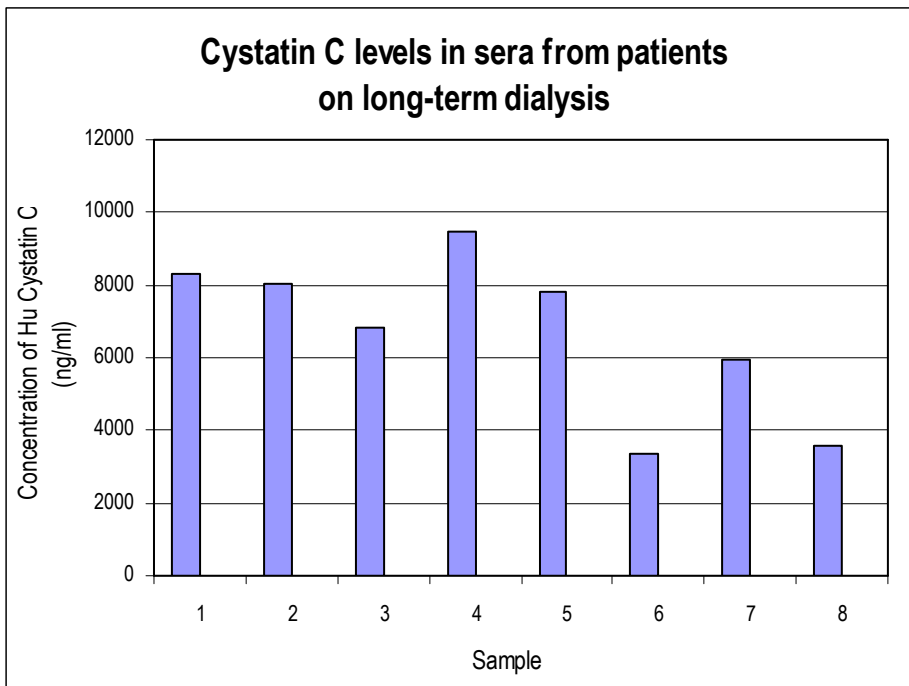


Figure 5: Cystatin C concentration was determined in serum samples from eight patients on long-term dialysis.

Sample No.	Cystatin C (ng/ml)	CV (%)
pooled serum	1 032	11
1	885	9
2	979	4
3	703	8
4	1 178	6
5	943	8
6	751	9
7	850	5
8	1 532	6
9	1 328	2

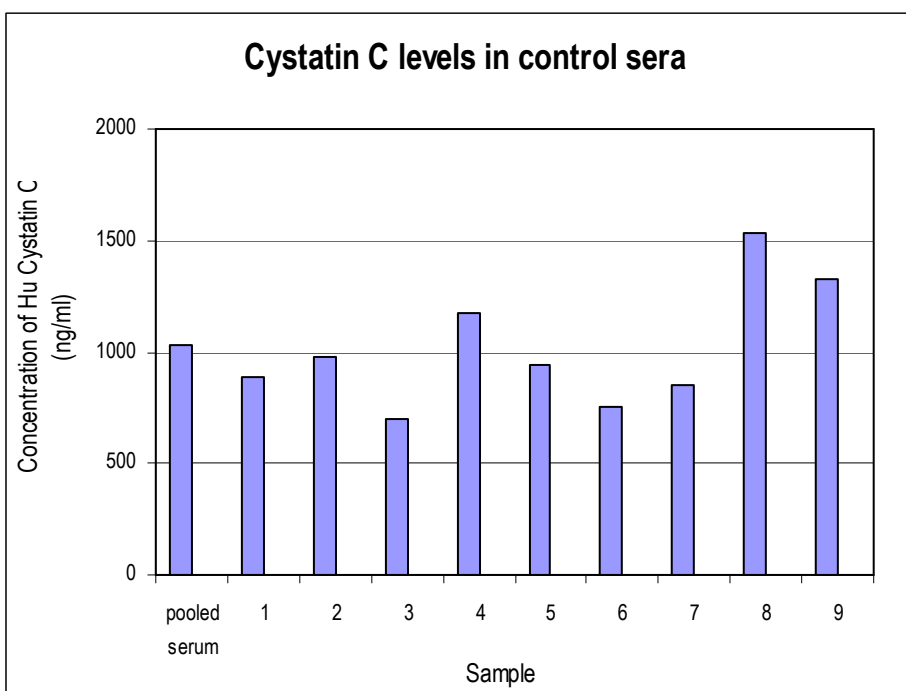



Figure 6: Samples from nine volunteers and a pooled serum were used as control sera.

- **Reference range**

The data quoted in these instructions should be used for guidance only. It is recommended that each laboratory include its own panel of control sample in the assay. Each laboratory should establish its own normal and pathological references ranges for cystatin C levels with the assay.

17. METHOD COMPARISON

The BioVendor Human Cystatin C ELISA was compared to the other commercial immunoturbidimetric assay, by measuring 38 serum samples. The following correlation graph was obtained.

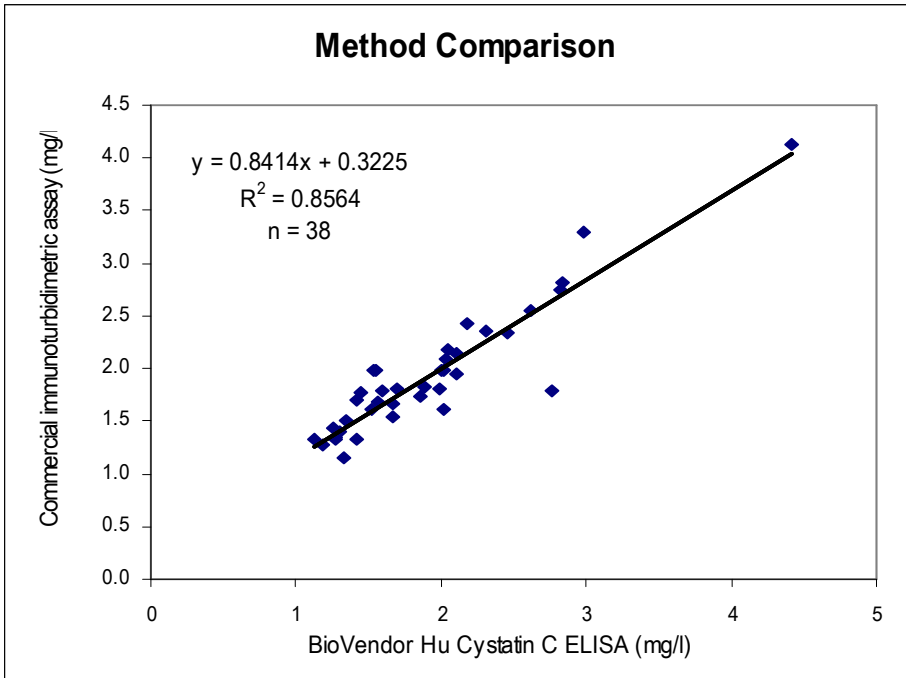

18. TROUBLESHOOTING AND FAQs

»» Weak signal in all wells

Possible explanations:

- Omission of a reagent or a step
- Improper preparation or storage of a reagent
- Assay performed before reagents were allowed to come to room temperature
- Improper wavelength when reading absorbance

»» High signal and background in all wells

Possible explanations:

- Improper or inadequate washing
- Overdeveloping; incubation time with Substrate Solution should be decreased before addition of Stop Solution
- Incubation temperature over 30°C

»» High coefficient of variation (CV)

Possible explanation:

- Improper or inadequate washing
- Improper mixing Standards, Quality Controls or samples

19. REFERENCES

»» References to cystatin C:

- Ekiel I, Abrahamson M, Fulton DB, Lindahl P, Storer AC, Levadoux W, Lafrance M, Labelle S, Pomerleau Y, Groleau D, LeSauter L, Gehring K: NMR structural studies of human cystatin C dimmers and monomers. *J Mol Biol.* **271**: 266-277 (1997)
- Tian S, Kusano E, Ohara T, Tabei K, Itoh Y, Kawai T, Asano Y: Cystatin C measurement and its practical use in patients with various renal diseases. *Clin Nephrol.* **48**: 104-108 (1997)
- Bokenkamp A, Domanetzki M, Zinck R, Schumann G, Byrd D, Brodehl J: Cystatin C – a new marker of glomerular filtration rate in children independent of age and height. *Pediatrics.* **101**: 875-881 (1998)
- Risch L, Blumberg A, Huber A: Rapid and accurate assessment of glomerular filtration rate in patients with renal transplants using serum cystatin C. *Nephrol Dial Transplant.* **14**: 1991-1996 (1999)
- Deng A, Irizarry MC, Nitsch RM, Growdon JH, Rebeck GW: Elevation of cystatin C in susceptible neurons in Alzheimer's disease. *Am J Pathol.* **159**: 1061-1068 (2001)
- Dharnidharka VR, Kwon C, Stevens G: Serum cystatin C is superior to serum creatinine as a marker of kidney function: a meta-analysis. *Am J Kidney Dis.* **40**: 221-226 (2002)
- Mojiminiyi OA and Abdella N: Evaluation of cystatin C and beta-2 microglobulin as markers of renal function in patients with type 2 diabetes mellitus. *J Diabetes Complications.* **17**: 160-168 (2003)
- Perlemoine C, Beauvieux MC, Rigalleau V, Baillet L, Barthes N, Derache P, Gin H: Interest of cystatin C in screening diabetic patients for early impairment of renal function. *Metabolism.* **52**: 1258-1264 (2003)
- Mussap M and Plebani M: Biochemistry and Clinical Role of Human Cystatin C. *Crit Rev Clin Lab Sci.* **41**: 467-550 (2004)
- Johnston N, Jernberg T, Lindahl B, Lindback J, Stridsberg M, Larsson A, Venge P, Wallentin L: Biochemical indicators of cardiac and renal function in a healthy elderly population. *Clin Biochem.* **37**: 210-216 (2004)
- Luc G, Bard JM, Lesueur C, Arveiler D, Evans A, Amouyel P, Ferrieres J, Juhan-Vague I, Fruchart JC, Ducimetiere P: Plasma cystatin-C and development of coronary heart disease: The PRIME Study. *Atherosclerosis.* (2005)
- Macisaac RJ, Tsalamandris C, Thomas MC, Premaratne E, Panagiotopoulos S, Smith TJ, Poon A, Jenkins MA, Ratnaik SI, Power DA, Jerums G: Estimating glomerular filtration rate in diabetes: a comparison of cystatin-C- and creatinine-based methods. *Diabetologia.* **49**: 1686-1689 (2006)
- Nakashima I, Fujihara K, Fujinoki M, Kawamura T, Nishimura T, Nakamura M, Itoyama Y: Alteration of cystatin C in the cerebrospinal fluid of multiple sclerosis. *Ann Neurol.* (2006)
- Delanaye P, Cavalier E, Krzesinski JM.: Cystatin C, renal function, and cardiovascular risk. *Ann Intern Med.* Jul **3**;147(1):19-27 (2007)










- Parikh NI, Hwang SJ, Yang Q, Larson MG, Guo CY, Robins SJ, Sutherland P, Benjamin EJ, Levy D, Fox CS: Clinical correlates and heritability of cystatin C (from the Framingham Offspring Study). *Am J Cardiol.* Nov 1;**102**(9):1194-8 (2008)
- Sundelöf J, Arnlöv J, Ingelsson E, Sundström J, Basu S, Zethelius B, Larsson A, Irizarry MC, Giedraitis V, Rönnekaa E, Degerman-Gunnarsson M, Hyman BT, Basun H, Kilander L, Lannfelt L: Serum cystatin C and the risk of Alzheimer disease in elderly men. *Neurology* Sep 30;**71**(14):1072-9 (2008)
- Ortiz F, Harmoinen A, Paavonen T, Koskinen P, Grönhagen-Riska C, Honkanen E: Is Cystatin C more sensitive than creatinine in detecting early chronic allograft nephropathy? *Clin Nephrol.* **70**(1):18-25 (2008)
- Samouilidou EC, Grapsa E.: Relationship of serum cystatin C with C-reactive protein and apolipoprotein A1 in patients on hemodialysis. *Ren Fail.* **30**(7):711-5(2008)
- Muntner P, Mann D, Winston J, Bansilal S, Farkouh ME.: Serum cystatin C and increased coronary heart disease prevalence in US adults without chronic kidney disease. *Am J Cardiol.* Jul 1;**102**(1):54-7 (2008)
- Servais A, Giral P, Bernard M, Bruckert E, Deray G, Isnard Bagnis C.: Is serum cystatin-C a reliable marker for metabolic syndrome? *Am J Med.* May;**121**(5):426-32 (2008)
- Muntner P, Winston J, Uribarri J, Mann D, Fox CS.: Overweight, obesity, and elevated serum cystatin C levels in adults in the United States. *Am J Med.* Apr;**121**(4):341-8 (2008)
- Premaratne E, Maclsaac RJ, Finch S, Panagiotopoulos S, Ekinci E, Jerums G.: Serial measurements of cystatin C are more accurate than creatinine-based methods in detecting declining renal function in type 1 diabetes. *Diabetes Care.* May;**31**(5):971-3 (2008).
- Moran A, Katz R, Smith NL, Fried LF, Sarnak MJ, Seliger SL, Psaty B, Siscovick DS, Gottdiener JS, Shlipak MG.: Cystatin C concentration as a predictor of systolic and diastolic heart failure. *J Card Fail.* Feb;**14**(1):19-26 (2008)

»» References to this product:


- Nedelkov D and Nelson RW: Delineating protein-protein interactions via biomolecular interaction analysis-mass spectrometry. *J Mol Recognit.* **16**: 9-14 (2003)
- Nedelkov D and Nelson RW: Design and use of multi-affinity surfaces in biomolecular interaction analysis-mass spectrometry (BIA/MS): a step toward the design of SPR/MS arrays. *J Mol Recognit.* **16**: 15-19 (2003)
- Mares J, Stejskal D, Vavrouskova J, Urbanek K, Herzig R, Hlustik P: Use of cystatin C determination in clinical diagnostics. *Biomed Papers.* **147**: 177-180 (2003)
- Straface E, Matarrese P, Gambardella L, Vona R, Sgadari A, Silveri MC, Malorni W: Oxidative imbalance and cathepsin D changes as peripheral blood biomarkers of Alzheimer disease: A pilot study. *FEBS Lett.* **579**: 2759-2766 (2005)
- Stejskal D, Vavrouskova J, Mares J, Urbanek K: Applications of new laboratory marker assays in neurological diagnoses - A pilot study. *Biomed Pap Med Fac Univ Palacky Olomouc Czech Repub.* **149**: 265-266 (2005)
- Taleb S, Lacasa D, Bastard JP, Poitou C, Canello R, Pelloux V, Viguerie N, Benis A, Zucker JD, Bouillot JL, Coussieu C, Basdevant A, Langin D, Clement K: Cathepsin S, a novel biomarker of adiposity: relevance to atherogenesis. *FASEB J.* **19**: 1540-1542 (2005)
- Barrientos LG, Rollin PE: Release of cellular proteases into the acidic extracellular milieu exacerbates Ebola virus-induced cell damage. *Virology* (2006)
- Liu XD, Zeng BF, Xu JG, Zhu HB, Xia QC: Proteomic analysis of the cerebrospinal fluid of patients with lumbar disk herniation. *Proteomics* **6**: 1019-1028 (2006)
- Yang X, Wang H, Wang Z, Dong M: Alteration and significance of serum cardiac troponin I and cystatin C in preeclampsia. *Clin Chim Acta.* **374**: 168-169 (2006)
- Taleb S, Canello R, Poitou C, Rouault C, Sellam P, Levy P, Bouillot JL, Coussieu C, Basdevant A, Guerre-Millo M, Lacasa D, Clement K: Weight loss reduces adipose tissue cathepsin S and its circulating levels in morbidly obese women. *J Clin Endocrinol Metab.* **91**: 1042-1047 (2006)
- Hossain M. A., Emara M., El moselhi. H., Shoker A.: Comparing measures of Cystatin C in human sera by three methods. *Am J Nephrology* **29(5)**: 381 – 391 (2009)
- Wilson M. E., Boumaza I., Lacomis D., Bowser R.: Cystatin : A candidate biomarker for amyotrophic lateral sclerosis. *PLoS ONE* **5(12)**: 1 – 9 (2010)
- Tanindi A., Olgun H., Tuncel A., Celik B., Pasaoglu H., Boyaci B.: Exercise electrocardiographic responses and serum cystatin C levels among metabolic syndrome patients without overt diabetes mellitus. *Vascular Health and Risk Management* **7**: 59 – 65 (2011)

»» For more references on this product see our WebPages at www.biovendor.com

20. EXPLANATION OF SYMBOLS

	Catalogue number
	Content
	Lot number
	See instructions for use
	Biological hazard
	Expiry date
	Storage conditions
	Identification of packaging materials
	In vitro diagnostic medical device

Assay Procedure Summary

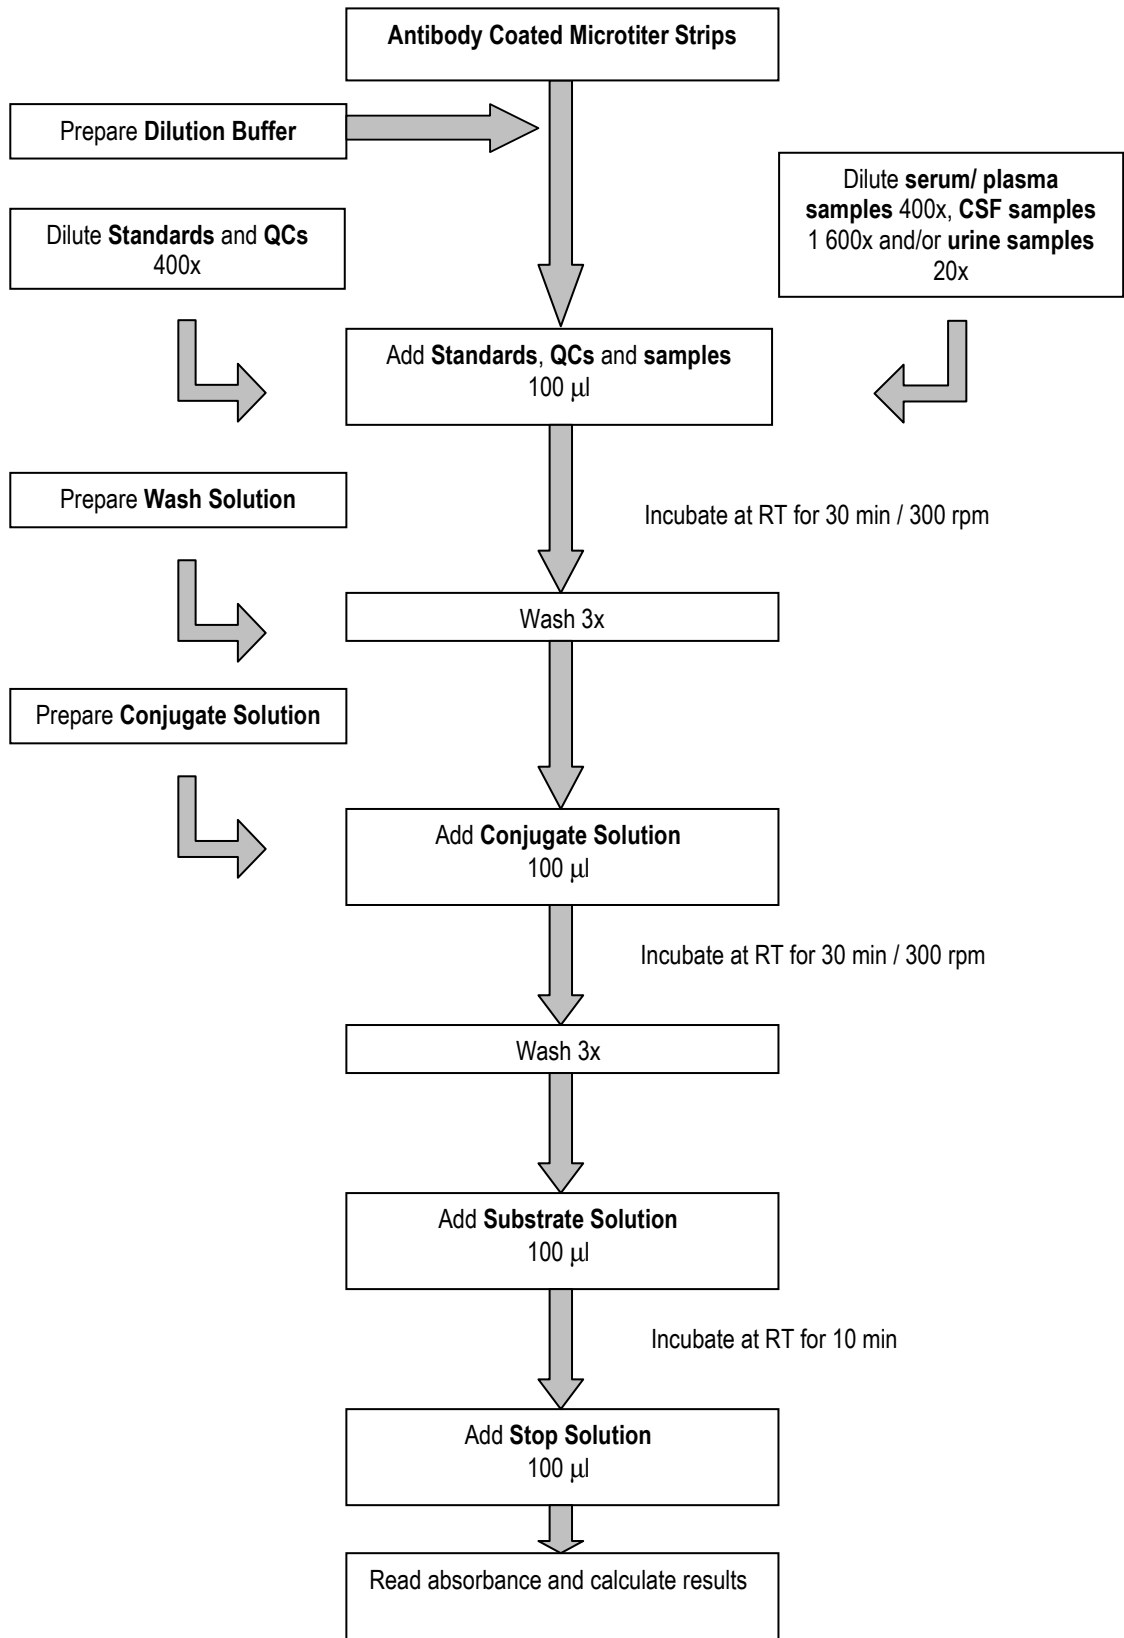


12								
11								
10								
9								
8								
7								
6								
5								
4								
3								
2								
1								
	A	B	C	D	E	F	G	H

NOTES



BioVendor

Research
and Diagnostic Products

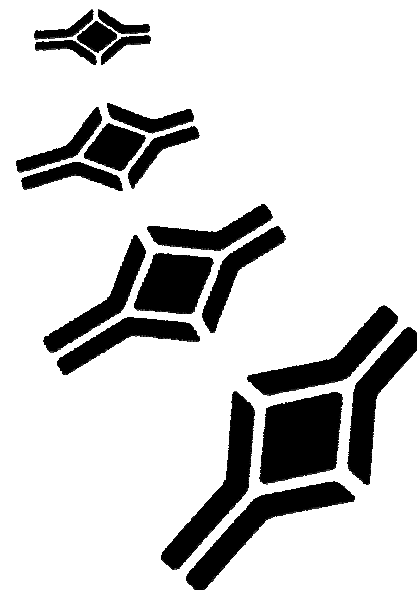

HEADQUARTERS:
BioVendor - Laboratorní
medicína a.s.

Karasek 1767/1

621 00 Brno
CZECH REPUBLIC

Phone: +420-549-124-185
Fax: +420-549-211-460

E-mail: info@biovendor.com
sales@biovendor.com
Web: www.biovendor.com

EUROPEAN UNION:
BioVendor GmbH

Im Neuenheimer Feld 583

D-69120 Heidelberg
GERMANY

Phone: +49-6221-433-9100
Fax: +49-6221-433-9111

E-mail: infoEU@biovendor.com

USA, CANADA AND MEXICO:
BioVendor LLC

128 Bingham Rd.
Suite 1300

Asheville, NC 28806
USA

Phone: +1-828-575-9250
+1-800-404-7807
Fax: +1-828-670-7809

E-mail: infoUSA@biovendor.com

CHINA - Hong Kong Office:
BioVendor Laboratories Ltd

Room 4008
Hong Kong Plaza, No.188

Connaught Road West
Hong Kong, CHINA

Phone: +852-2803-0523
Fax: +852-2803-0525

E-mail: infoHK@biovendor.com

CHINA – Mainland Office:
BioVendor Laboratories Ltd

Room 2917, 29/F
R & F Ying Feng Plaza, No.2
Huaqiang road

Pearl River New Town
Guang Zhou, CHINA

Phone: +86-20-38065519
Fax: +86-20-38065529

E-mail: infoCN@biovendor.com