


BioVendor

Research
and Diagnostic Products

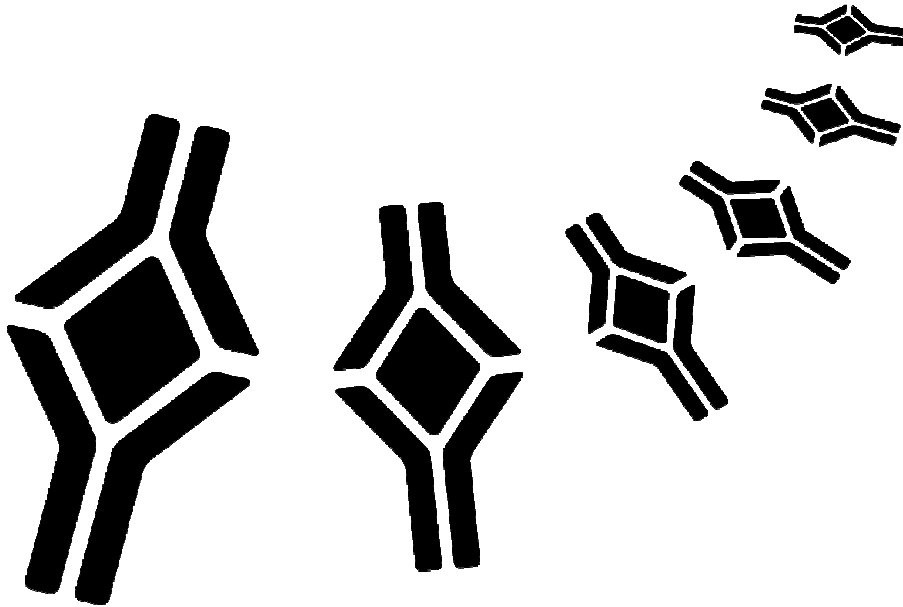

HUMAN PHOSPHORYLATED NEUROFILAMENT H ELISA

Product Data Sheet

Cat. No.: RD191138300R

For Research Use Only

CONTENTS

1.	INTENDED USE	3
2.	STORAGE, EXPIRATION	3
3.	INTRODUCTION	4
4.	TEST PRINCIPLE	5
5.	PRECAUTIONS	5
6.	TECHNICAL HINTS	6
7.	REAGENT SUPPLIED	6
8.	MATERIAL REQUIRED BUT NOT SUPPLIED	7
9.	PREPARATION OF REAGENTS	7
10.	PREPARATION OF SAMPLES	9
11.	ASSAY PROCEDURE	10
12.	CALCULATIONS	12
13.	PERFORMANCE CHARACTERISTICS	13
14.	DEFINITION OF THE STANDARD	16
15.	METHOD COMPARISON	16
16.	TROUBLESHOOTING AND FAQs	17
17.	REFERENCES	18
18.	EXPLANATION OF SYMBOLS	19

➤➤ **This kit is manufactured by:**
BioVendor – Laboratorní medicína a.s.

➤➤ **Use only the current version of Product Data Sheet enclosed with the kit!**

1. INTENDED USE

The RD191138300R Human Phosphorylated Neurofilament H ELISA is a sandwich enzyme immunoassay for the quantitative measurement of human phosphorylated neurofilament H (pNF-H).

»» Features

- **It is intended for research use only**
- The total assay time is less than 4 hours
- The kit measures pNF-H in serum, plasma and cerebrospinal fluid (CSF)
- Assay format is 96 wells
- Standard and Quality Controls are human brain extract based
- Components of the kit are provided ready to use, concentrated or lyophilized

2. STORAGE, EXPIRATION

Store the complete kit at 2-8°C. Under these conditions, the kit is stable until the expiration date (see label on the box).

For stability of opened reagents see Chapter 9.

3. INTRODUCTION

Neurofilaments are the 10nm diameter filaments which are the most abundant protein components of neurons and are particularly concentrated in axons. They belong to the intermediate or 10nm filament protein/gene superfamily which also includes keratins, the major structural proteins of skin. Neurofilaments (NF) consist predominantly of three subunits: NF-L (low), NF-M (medium), and NF-H (heavy or high). NF-H protein is about 200 kDa and contains unusual multiple repeated sequence lysine-serine-proline (KSP), and in axonal neurofilaments essentially all serine residues are heavily phosphorylated. Because phosphorylated forms of NF-H (pNF-H) are quite resistant to proteases, pNF-H released from damaged and diseased axons should remain in fluid undegraded. This means that detection of pNF-H in blood and CSF points unambiguously to neuronal damage due to the fact that pNF-H is found exclusively in neurons.

This protein can be detected in quite large amounts following experimental spinal cord and brain injury in rats. Levels of greater than 100 ng/ml of pNF-H were detectable in blood following serious cord injury and lower, but still easily detectable levels, were found in blood of animals given experimental brain injury. In recently studies with rats subjected to traumatic brain injury (TBI) using a controlled cortical impact (CCI) device, elevated blood pNF-H levels were found. Results show time-dependent changes in the detectable pNF-H levels and these levels correspond with the severity of the injury and the amount of cortical damage.

Studies with mice transgenic for mutations of human copper/zinc superoxide dismutase 1 which are associated with amyotrophic lateral sclerosis (ALS) have revealed corresponding increased amounts of pNF-H in blood of these animals. These mice develop axonal degeneration pathology similar to that seen in humans with ALS, and blood pNF-H levels can be used to monitor this degeneration. Interestingly, pNF-H is detectable before the onset of obvious disease symptoms.

Other experiments have shown that pNF-H is detected in the plasma of humans suffering from optic neuritis and in elevated levels in the cerebrospinal fluid (CSF) of individuals suffering from brain tumors and stroke.

Areas of investigation:

Axonal degeneration

Brain injury

Neuronal damage

4. TEST PRINCIPLE

In the BioVendor Human Phosphorylated Neurofilament H ELISA, standards, quality controls and samples are incubated in microplate wells pre-coated with chicken polyclonal anti-pNF-H antibody. After 60 minutes incubation and washing, detection rabbit polyclonal anti-pNF-H antibody is added and incubated with captured pNF-H for 60 minutes. After another washing, HRP conjugated antibody against rabbit antibody is added. After 60 minutes incubation and the last washing step, the remaining conjugate is allowed to react with the substrate solution (TMB). The reaction is stopped by addition of acidic solution and absorbance of the resulting yellow product is measured. The absorbance is proportional to the concentration of pNF-H. A standard curve is constructed by plotting absorbance values against concentrations of standards, and concentrations of unknown samples are determined using this standard curve.

5. PRECAUTIONS

- **For professional use only**
- Wear gloves and laboratory coats when handling immunodiagnostic materials
- Do not drink, eat or smoke in the areas where immunodiagnostic materials are being handled
- This kit contains components of human origin. These materials were found non-reactive for HBsAg, HCV antibody and for HIV 1/2 antigen and antibody. However, these materials should be handled as potentially infectious, as no test can guarantee the complete absence of infectious agents
- This kit contains components of animal origin. These materials should be handled as potentially infectious
- Avoid contact with the acidic Stop Solution and Substrate Solution, which contains hydrogen peroxide and tetramethylbenzidine (TMB). Wear gloves and eye and clothing protection when handling these reagents. Stop and/or Substrate Solutions may cause skin/eyes irritation. In case of contact with the Stop Solution and the Substrate Solution wash skin/eyes thoroughly with water and seek medical attention, when necessary
- The materials must not be pipetted by mouth

6. TECHNICAL HINTS

- Reagents with different lot numbers should not be mixed
- Use thoroughly clean glassware
- Use deionized (distilled) water, stored in clean containers
- Avoid any contamination among samples and reagents. For this purpose, disposable tips should be used for each sample and reagent
- Substrate Solution should remain colourless until added to the plate. Keep Substrate Solution protected from light
- Stop Solution should remain colourless until added to the plate. The colour developed in the wells will turn from blue to yellow immediately after the addition of the Stop Solution. Wells that are green in colour indicate that the Stop Solution has not mixed thoroughly with the Substrate Solution
- Dispose of consumable materials and unused contents in accordance with applicable national regulatory requirements

7. REAGENT SUPPLIED

<i>Kit Components</i>	<i>State</i>	<i>Quantity</i>
Antibody Coated Microtiter Strips	ready to use	96 wells
Detection Antibody Solution	ready to use	13 ml
HRP Conjugate Solution	ready to use	13 ml
Master Standard	lyophilized	2 vials
Quality Control HIGH	lyophilized	2 vials
Quality Control LOW	lyophilized	2 vials
Dilution Buffer	ready to use	13 ml
Wash Solution Conc. (10x)	concentrated	100 ml
Substrate Solution	ready to use	13 ml
Stop Solution	ready to use	13 ml
Product Data Sheet + Certificate of Analysis	-	1 pc

8. MATERIAL REQUIRED BUT NOT SUPPLIED

- Deionized (distilled) water
- Test tubes for diluting samples
- Glassware (graduated cylinder and bottle) for Wash Solution (Dilution Buffer)
- Precision pipettes to deliver 10-1000 μ l with disposable tips
- Multichannel pipette to deliver 100 μ l with disposable tips
- Absorbent material (e.g. paper towels) for blotting the microtiter plate after washing
- Vortex mixer
- Orbital microplate shaker capable of approximately 300 rpm
- Microplate washer (optional). [Manual washing is possible but not preferable]
- Microplate reader with 450 ± 10 nm filter, preferably with reference wavelength 630 nm (alternatively another one from the interval 550-650 nm)
- Software package facilitating data generation and analysis (optional)

9. PREPARATION OF REAGENTS

- All reagents need to be brought to room temperature prior to use
- Always prepare only the appropriate quantity of reagents for your test
- Do not use components after the expiration date marked on their label

- Assay reagents supplied ready to use:

Antibody Coated Microtiter Strips

Stability and storage:

Return the unused strips to the provided aluminium zip-sealed bag with desiccant and seal carefully. Remaining Microtiter Strips are stable 3 months stored at 2-8°C and protected from the moisture.

Detection Antibody Solution

HRP Conjugate Solution

Dilution Buffer

Substrate Solution

Stop Solution

Stability and storage:

Opened reagents are stable 3 months when stored at 2-8°C.

- **Assay reagents supplied concentrated or lyophilized:**

pNF-H Master Standard

Refer to the Certificate of Analysis for current volume of Dilution Buffer needed for reconstitution of standard!!!

Reconstitute the lyophilized Master Standard with Dilution Buffer just prior to the assay. Let it dissolve at least 15 minutes with occasional gentle shaking (not to foam). The resulting concentration of the pNF-H in the stock solution is **4 000 pg/ml**.

Prepare set of standards using Dilution Buffer as follows:

<i>Volume of Standard</i>	<i>Dilution Buffer</i>	<i>Concentration</i>
Stock	-	4 000 pg/ml
250 µl of stock	250 µl	2 000 pg/ml
250 µl of 2 000 pg/ml	250 µl	1 000 pg/ml
250 µl of 1 000 pg/ml	250 µl	500 pg/ml
250 µl of 500 pg/ml	250 µl	250 pg/ml
250 µl of 250 pg/ml	250 µl	125 pg/ml
250 µl of 125 pg/ml	250 µl	62.5 pg/ml

Prepared Standards are ready to use, do not dilute them.

Stability and storage:

Do not store the Standard stock solution and set of standards.

Quality Controls HIGH, LOW

Refer to the Certificate of Analysis for current volume of Dilution Buffer needed for reconstitution and for current Quality Control concentration!!!

Reconstitute each Quality Control (HIGH and LOW) with Dilution Buffer just prior to the assay. Let it dissolve at least 15 minutes with occasional gentle shaking (not to foam).

Reconstituted Quality Controls are ready to use, do not dilute them.

Stability and storage:

Do not store the reconstituted Quality Controls.

Note:

Concentration of analyte in Quality Controls need not be anyhow associated with normal and/or pathological concentrations in serum or another body fluid. Quality Controls serve just for control that the kit works in accordance with PDS and CoA and that ELISA test was carried out properly.

Wash Solution Conc. (10x)

Dilute Wash Solution Concentrate (10x) ten-fold in distilled water to prepare a 1x working solution. Example: 100 ml of Wash Solution Concentrate (10x) + 900 ml of distilled water for use of all 96-wells.

Stability and storage:

The diluted Wash Solution is stable 1 month when stored at 2-8°C. Opened Wash Solution Concentrate (10x) is stable 3 months when stored at 2-8°C.

10. PREPARATION OF SAMPLES

The kit measures pNF-H in human serum, plasma and CSF.

Samples should be assayed immediately after collection or should be stored at -20°C. Mix thoroughly thawed samples just prior to the assay and avoid repeated freeze/thaw cycles, which may cause erroneous results. Avoid using hemolyzed or lipemic samples.

Dilute samples 3x with Dilution Buffer just prior to the assay, e.g. 50 µl of sample + 100 µl of Dilution Buffer for singlets, or preferably 80 µl of sample + 160 µl of Dilution Buffer for duplicates. **Mix well** (not to foam). Vortex is recommended.

Stability and storage:

Serum and plasma samples should be stored at -20°C, or preferably at -70°C for long-term storage. CSF samples should be stored at -70°C.

Do not store the diluted samples.

See Chapter 13 for stability of serum and CSF samples when stored at 2-8°C and effect of freezing/thawing on the concentration of human pNF-H.

Note: It is recommended to use a precision pipette and a careful technique to perform the dilution in order to get precise results.

11. ASSAY PROCEDURE

1. Pipet **100 µl** of diluted Standards, Quality Controls, Dilution Buffer (=Blank) and samples, preferably in duplicates, into the appropriate wells. See *Figure 1* for example of work sheet.
2. Incubate the plate at room temperature (ca. 25°C) for **1 hour**, shaking at ca. 300 rpm on an orbital microplate shaker.
3. Wash the wells 3-times with Wash Solution (0.35 ml per well). After final wash, invert and tap the plate strongly against paper towel.
4. Add **100 µl** of Detection Antibody Solution into each well.
5. Incubate the plate at room temperature (ca. 25°C) for **1 hour**, shaking at ca. 300 rpm on an orbital microplate shaker.
6. Wash the wells 3-times with Wash Solution (0.35 ml per well). After final wash, invert and tap the plate strongly against paper towel.
7. Add **100 µl** of HRP Conjugate Solution into each well.
8. Incubate the plate at room temperature (ca. 25°C) for **1 hour**, shaking at ca. 300 rpm on an orbital microplate shaker.
9. Wash the wells 3-times with Wash Solution (0.35 ml per well). After final wash, invert and tap the plate strongly against paper towel.
10. Add **100 µl** of Substrate Solution into each well. Avoid exposing the microtiter plate to direct sunlight. Covering the plate with e.g. aluminium foil is recommended.
11. Incubate the plate for **15 minutes** at room temperature. The incubation time may be extended [up to 25 minutes] if the reaction temperature is below than 20°C. Do not shake the plate during the incubation.
12. Stop the colour development by adding **100 µl** of Stop Solution.
13. Determine the absorbance of each well using a microplate reader set to 450 nm, preferably with the reference wavelength set to 630 nm (acceptable range: 550 - 650 nm). Subtract readings at 630 nm (550 - 650 nm) from the readings at 450 nm. **The absorbance should be read within 5 minutes following step 12.**

Note: If some samples and standard/s have absorbances above the upper limit of your microplate reader, perform a second reading at 405 nm. A new standard curve, constructed using the values measured at 405 nm, is used to determine pNF-H concentration of off-scale standards and samples. The readings at 405 nm should not replace the readings for samples that were "in range" at 450 nm.

Note 2: Manual washing: Aspirate wells and pipet 0.35 ml Wash Solution into each well. Aspirate wells and repeat twice. After final wash, invert and tap the plate strongly against paper towel. Make certain that Wash Solution has been removed entirely.

	strip 1+2	strip 3+4	strip 5+6	strip 7+8	strip 9+10	strip 11+12
A	Standard 4 000	QC HIGH	Sample 7	Sample 15	Sample 23	Sample 31
B	Standard 2 000	QC LOW	Sample 8	Sample 16	Sample 24	Sample 32
C	Standard 1 000	Sample 1	Sample 9	Sample 17	Sample 25	Sample 33
D	Standard 500	Sample 2	Sample 10	Sample 18	Sample 26	Sample 34
E	Standard 250	Sample 3	Sample 11	Sample 19	Sample 27	Sample 35
F	Standard 125	Sample 4	Sample 12	Sample 20	Sample 28	Sample 36
G	Standard 62.5	Sample 5	Sample 13	Sample 21	Sample 29	Sample 37
H	Blank	Sample 6	Sample 14	Sample 22	Sample 30	Sample 38

Figure 1: Example of a work sheet.

12. CALCULATIONS

Most microplate readers perform automatic calculations of analyte concentration. The standard curve is constructed by plotting the mean absorbance (Y) of Standards against the known concentration (X) of Standards in logarithmic scale, using the four-parameter algorithm. Results are reported as concentration of pNF-H pg/ml in samples.

Alternatively, the *logit log* function can be used to linearize the standard curve, i.e. *logit* of the mean absorbance (Y) is plotted against log of the known concentration (X) of Standards).

The measured concentration of samples calculated from the standard curve must be multiplied by their respective dilution factor, because samples have been diluted prior to the assay, e.g. 400 pg/ml (from standard curve) x 3 (dilution factor) = 1 200 pg/ml = 1.2 ng/ml.

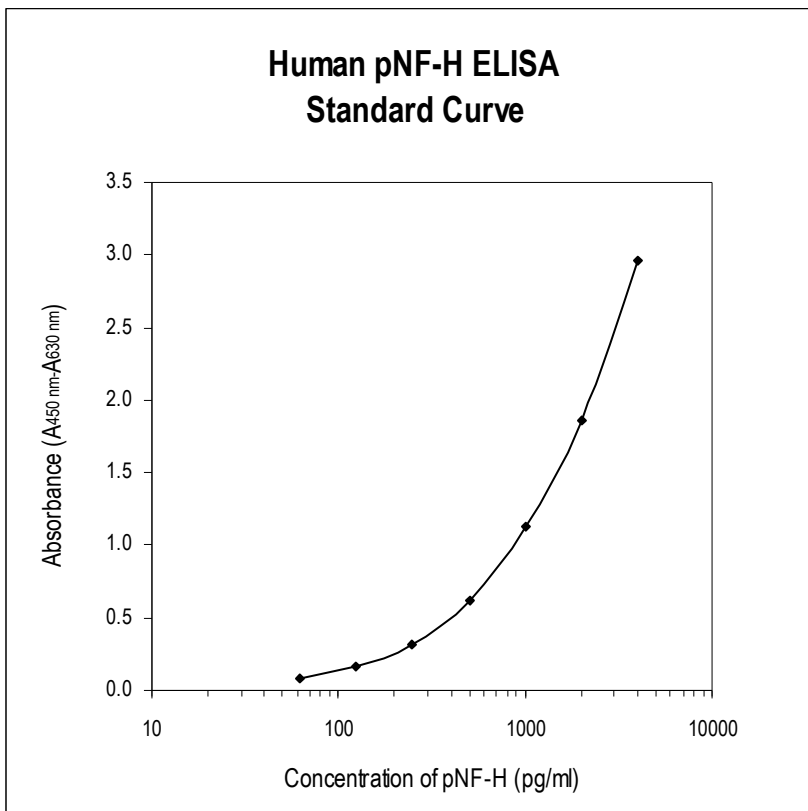


Figure 2: Typical Standard Curve for Human pNF-H ELISA.

13. PERFORMANCE CHARACTERISTICS

➤➤ Typical analytical data of BioVendor Human pNF-H ELISA are presented in this chapter

- **Sensitivity**

Limit of Detection (LOD) (defined as concentration of analyte giving absorbance higher than mean absorbance of blank* plus three standard deviations of the absorbance of blank: $A_{\text{blank}} + 3 \times \text{SD}_{\text{blank}}$) is calculated from the real pNF-H values in wells and is 23.5 pg/ml.

*Dilution Buffer is pipetted into blank wells.

- **Limit of assay**

Results exceeding pNF-H level of 4 000 pg/ml should be repeated with more diluted samples. Dilution factor needs to be taken into consideration in calculating the pNF-H concentration.

- **Specificity**

The antibodies used in this ELISA are specific for pNF-H from human and from mammalian species such as mouse, rat, rabbit, dog, pig, horse and bovine.

For details please contact us at info@biovendor.com.

➤➤ Presented results are multiplied by respective dilution factor

- **Precision**

Intra-assay (Within-Run) (n=8)

<i>CSF sample</i>	<i>Mean (pg/ml)</i>	<i>SD (pg/ml)</i>	<i>CV (%)</i>
1	963	48.2	5.0
2	1 829	73.2	4.0

Inter-assay (Run-to-Run) (n=8)

<i>CSF sample</i>	<i>Mean (pg/ml)</i>	<i>SD (pg/ml)</i>	<i>CV (%)</i>
1	1 410	64.1	4.5
2	3 212	76.9	2.4

- **Spiking Recovery**

CSF and serum samples were spiked with different amounts of pNF-H and assayed.

<i>CSF sample</i>	<i>Observed (pg/ml)</i>	<i>Expected (pg/ml)</i>	<i>Recovery O/E (%)</i>
1	985	-	-
	3 672	3 985	92.1
	2 713	2 485	109.2
	1 608	1 735	92.7
2	2 046	-	-
	2 572	2 796	92.0
	3 519	3 546	99.2
	5 419	5 046	107.4

<i>Serum sample</i>	<i>Observed (pg/ml)</i>	<i>Expected (pg/ml)</i>	<i>Recovery O/E (%)</i>
1	1 648	-	-
	2 180	2 398	90.2
	3 028	3 148	96.2
	4 863	4 648	104.6
2	2 128	-	-
	2 618	2 878	99.3
	3 399	3 628	93.7
	5 090	5 128	91.0

- **Linearity**

CSF and serum samples were serially diluted with Dilution Buffer and assayed.

<i>CSF sample</i>	<i>Dilution</i>	<i>Observed (pg/ml)</i>	<i>Expected (pg/ml)</i>	<i>Recovery O/E (%)</i>
1	-	3 576	-	-
	2x	1 804	1 788	100.9
	4x	933	894	104.3
	8x	440	447	98.4
2	-	13 791	-	-
	2x	7 664	6 894	111.1
	4x	3 822	3 448	110.9
	8x	1 918	1 724	111.2

<i>Serum sample</i>	<i>Dilution</i>	Observed <i>(pg/ml)</i>	Expected <i>(pg/ml)</i>	Recovery O/E (%)
1	-	3 333	-	-
	2x	1 629	1 667	97.7
	4x	859	833	103.0
	8x	390	417	93.7
2	-	16 499	-	-
	2x	9 209	8 249	111.6
	4x	4 773	4 125	115.7
	8x	2 293	2 062	111.2

- **Stability of samples stored at 2-8°C**

Samples should be stored at -20°C. However, no decline in concentration of pNF-H was observed in CSF and serum samples after 7 days when stored at 2-8°C. To avoid microbial contamination, samples were treated with ε-aminocaproic acid and sodium azide, resulting in the final concentration of 0.03% and 0.1%, respectively.

<i>CSF sample</i>	<i>Incubation Temp, Period</i>	<i>pNF-H</i> <i>(pg/ml)</i>
1	-20°C	785
	2-8°C, 1 day	778
	2-8°C, 7 days	750
2	-20°C	2 633
	2-8°C, 1 day	2 684
	2-8°C, 7 days	2 605
3	-20°C	4 439
	2-8°C, 1 day	4 363
	2-8°C, 7 days	4 074

<i>Serum sample</i>	<i>Incubation Temp, Period</i>	<i>pNF-H</i> <i>(pg/ml)</i>
1	-20°C	370
	2-8°C, 1 day	434
	2-8°C, 7 days	385
2	-20°C	1 591
	2-8°C, 1 day	1 561
	2-8°C, 7 days	1 356
3	-20°C	3 333
	2-8°C, 1 day	2 901
	2-8°C, 7 days	3 003

- **Effect of Freezing/Thawing**

No decline was observed in concentration of human pNF-H in CSF and serum samples after repeated (5x) freeze/thaw cycles. However it is recommended to avoid unnecessary repeated freezing/thawing of the samples.

<i>CSF sample</i>	<i>Number of f/t cycles</i>	<i>pNF-H (pg/ml)</i>
1	1x	778
	3x	726
	5x	779
2	1x	2 585
	3x	2 663
	5x	2 660
3	1x	4 235
	3x	4 265
	5x	4 048

<i>Serum sample</i>	<i>Number of f/t cycles</i>	<i>pNF-H (pg/ml)</i>
1	1x	440
	3x	329
	5x	329
2	1x	1 608
	3x	1 695
	5x	1 669
3	1x	3 124
	3x	3 017
	5x	2 956

14. DEFINITION OF THE STANDARD

Standard in this assay is human brain extract based. Native pNF-H is about 200 kDa protein.

15. METHOD COMPARISON

BioVendor Human pNF-H ELISA was not compared to any other commercial immunoassay.

16. TROUBLESHOOTING AND FAQs

➤➤ Weak signal in all wells

Possible explanations:

- Omission of a reagent or a step
- Improper preparation or storage of a reagent
- Assay performed before reagents were allowed to come to room temperature
- Improper wavelength when reading absorbance

➤➤ High signal and background in all wells

Possible explanations:

- Improper or inadequate washing
- Overdeveloping; incubation time with Substrate Solution should be decreased before addition of Stop Solution
- Incubation temperature over 30°C

➤➤ High coefficient of variation (CV)

Possible explanation:

- Improper or inadequate washing
- Improper mixing Standards, Quality Controls or samples

17. REFERENCES

»» References to pNF-H:









- Anderson KJ, Sheff SW, Miller KM, Roberts KN, Gilmer LK, Yang C, and Shaw G: The Phosphorylated Axonal Form of the Neurofilament Subunit NF-H (pNF-H) as a Blood Biomarker of Traumatic Brain Injury. *J Neurot.* 2008; 25:1079-1085
- Lewis SB, Wolper RA, Miralia L, Yang C, Shaw G. Detection of phosphorylated NF-H in the cerebrospinal fluid and blood of aneurysmal subarachnoid hemorrhage patients. *J Cereb Blood Flow Metab.* 2008; 28(6):1261-71.
- Petzold A, Shaw G: Comparison of two ELISA methods for measuring levels of the phosphorylated neurofilament heavy chain. *J Immunol Methods* 2007; 319:34-40
- Shaw G, Lewis SB, Wolper R, Weiss M, Anderson K, Yang C, Wang Y, Borchelt D, Howland D: Recent studies of phosphorylated neurofilament nf-h (pnf-h) as a biomarker of axonal injury and degeneration. Georgia World Congress Center. 2006; Oct 18
- Petzold A: Neurofilament phosphoforms: surrogate markers for axonal injury, degeneration and loss. *J Neurol Sci.* 2005; 233 (1-2):183-98
- Shaw G, Yang C, Ellis R, Anderson K, Mickle JP, Scheff S, Pike B, Anderson DK, Howland DR. Hyperphosphorylated neurofilament NF-H is a serum biomarker of axonal injury. *Biochem Biophys Res Commun.* 2005; 336: 1268-1277
- Petzold A, Rejdak K, and Plant GT: Axonal degeneration and inflammation in acute optic neuritis. *J Neurol Neurosurg Psychiatry* 2004; 75:1178-80
- Hu YY, He SS, Wang XC, Duan QH, Khatoun S, Iqbal K, Grundke-Iqbal I, Wang JZ: Elevated levels of phosphorylated neurofilament proteins in cerebrospinal fluid of Alzheimer disease patients. *Neurosci Lett.* 2002; 320:156-60

»» References to this product:


- Žurek J, Bartlová L and Fedora M: Hyperphosphorylated neurofilament NF-H as a predictor of mortality after brain injury in children. *Brain Injury* 2011, 25(2) : 221-226

»» For more references on this product see our WebPages at www.biovendor.com

18. EXPLANATION OF SYMBOLS


	Catalogue number
	Content
	Lot number
	See instructions for use
	Biological hazard
	Expiry date
	Storage conditions
	Identification of packaging materials


Assay Procedure Summary

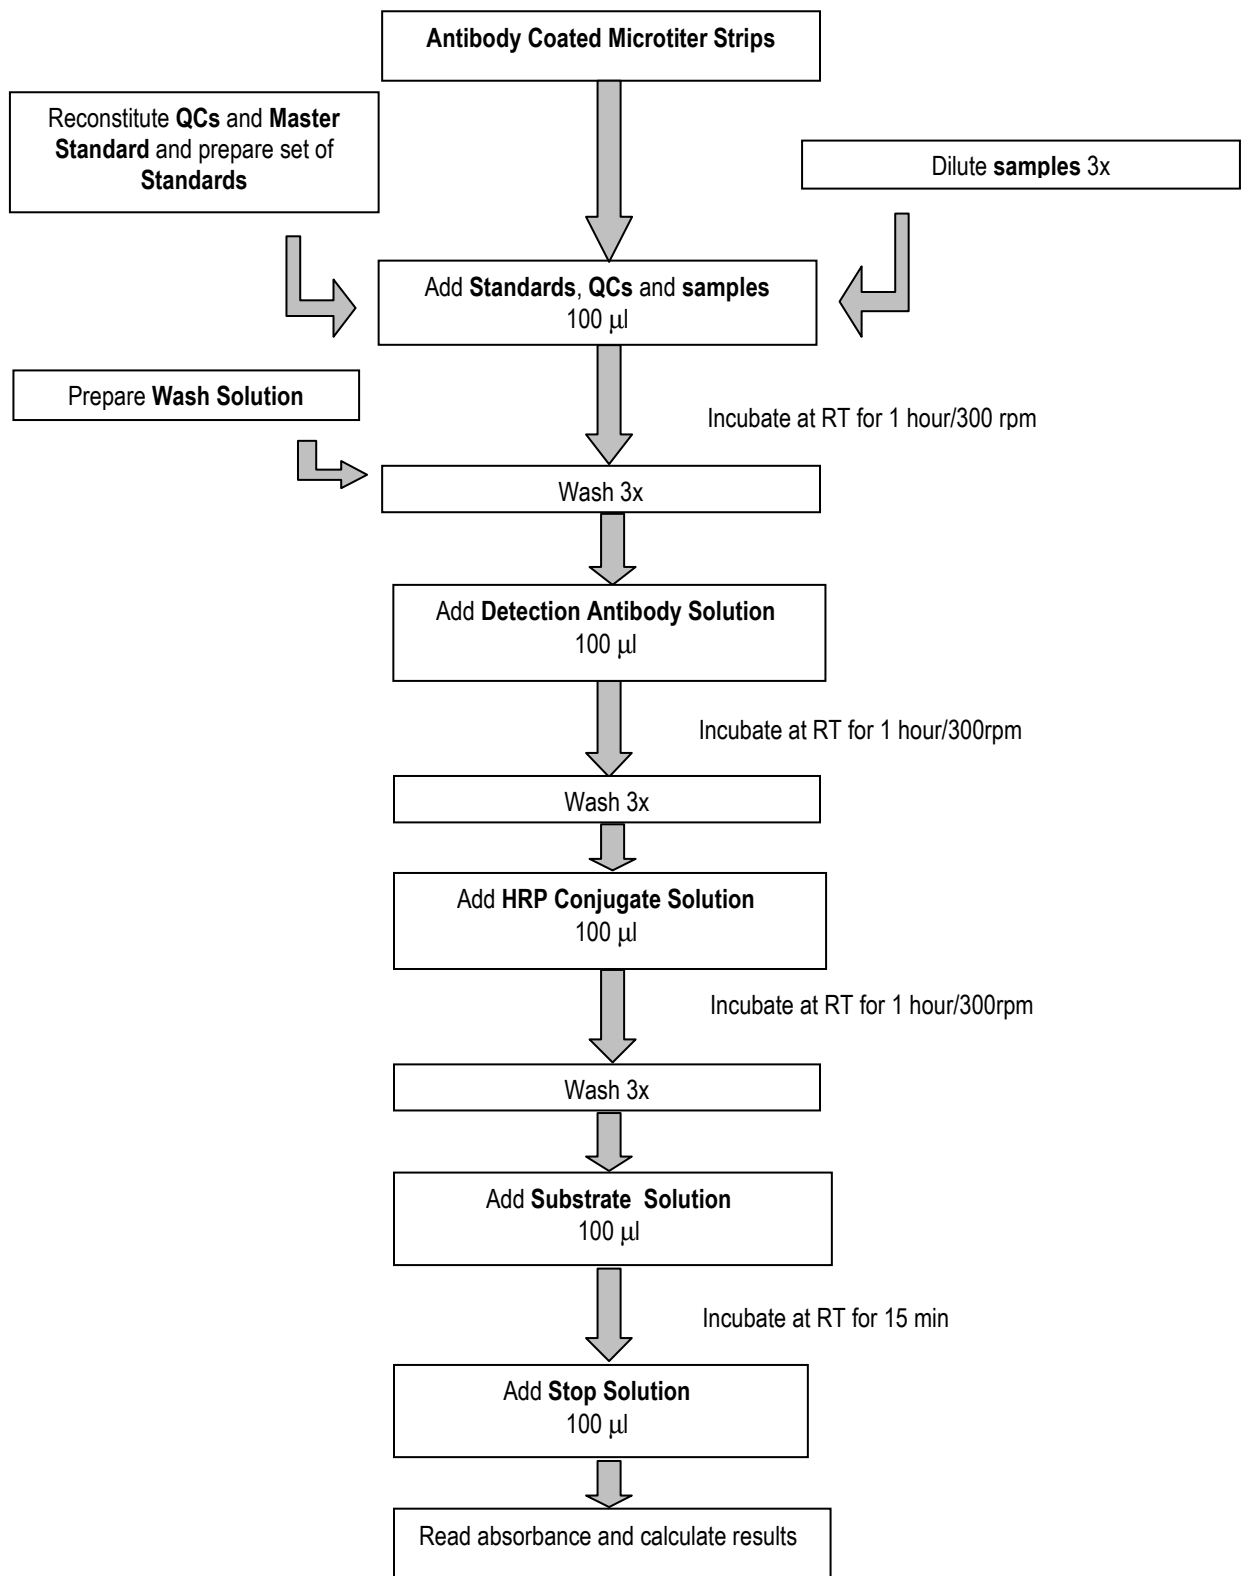

12								
11								
10								
9								
8								
7								
6								
5								
4								
3								
2								
1								
	A	B	C	D	E	F	G	H

NOTES



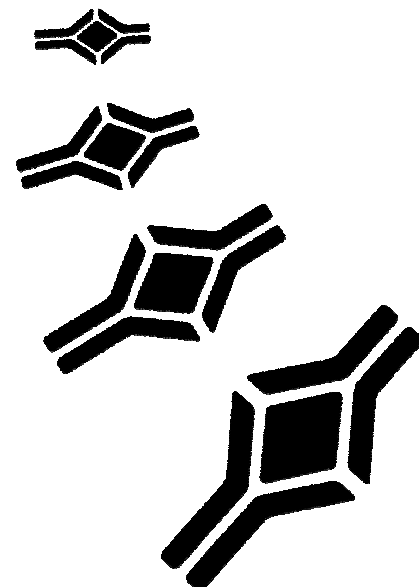

HEADQUARTERS: BioVendor- Laboratorní medicína a.s.	Karasek 1767/1	621 00 Brno CZECH REPUBLIC	Phone: +420-549-124-185 Fax: +420-549-211-460	E-mail: info@biovendor.com sales@biovendor.com Web: www.biovendor.com
EUROPEAN UNION: BioVendor GmbH	Im Neuenheimer Feld 583	D-69120 Heidelberg GERMANY	Phone: +49-6221-433-9100 Fax: +49-6221-433-9111	E-mail: infoEU@biovendor.com
USA, CANADA AND MEXICO: BioVendor LLC	128 Bingham Rd. Suite 1300	Asheville, NC 28806 USA	Phone: +1-828-575-9250 +1-800-404-7807 Fax: +1-828-575-9251	E-mail: infoUSA@biovendor.com
CHINA - Hong Kong Office: BioVendor Laboratories Ltd	Room 4008 Hong Kong Plaza, No.188	Connaught Road West Hong Kong, CHINA	Phone: +852-2803-0523 Fax: +852-2803-0525	E-mail: infoHK@biovendor.com
CHINA – Mainland Office: BioVendor Laboratories Ltd	Room 2917, 29/F R & F Ying Feng Plaza No.2 Huagiang road	Pearl River New Town Guang Zhou, CHINA	Phone: +86-20-38065519 Fax: +86-20-38065529	E-mail: infoCN@biovendor.com